

Mass Spectrum List Report

Analysis Info

Analysis Name D:\Data\ggc\24-121832_P1-B-1_01_9879.d
 Method lc-ms directos tunelow261224 apci.m
 Sample Name 24-121832
 Comment AR2F2
 Sv: MeOH + HCOOH
 Manuela García


Acquisition Date 12/26/2024 3:16:28 PM

Operator EB - MV

Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	APCI	Ion Polarity	Positive	Set Nebulizer	1.6 Bar
Focus	Not active	Set Capillary	4500 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	8.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

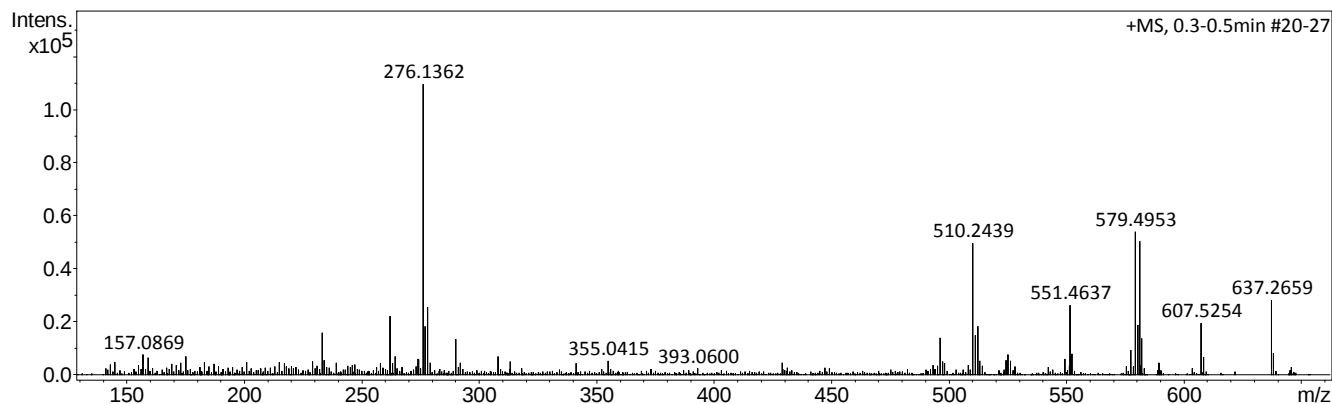

#	m/z	I	I %
1	157.0869	7874	7.2
2	159.0986	6595	6.0
3	175.0966	7080	6.5
4	233.1003	15944	14.6
5	262.1567	22208	20.3
6	264.1338	7029	6.4
7	274.1221	6051	5.5
8	274.2518	5921	5.4
9	276.1362	109487	100.0
10	277.1391	18457	16.9
11	278.1496	25618	23.4
12	290.1164	13513	12.3
13	308.1298	7126	6.5
14	496.2609	14081	12.9
15	510.2439	49566	45.3
16	511.2481	15000	13.7
17	512.2600	18226	16.6
18	525.1476	7775	7.1
19	549.4382	6042	5.5
20	551.4637	26302	24.0
21	552.4659	7981	7.3
22	577.4692	9442	8.6
23	579.4953	53864	49.2
24	580.4977	18788	17.2
25	581.2046	50201	45.9
26	582.2065	13809	12.6
27	607.5254	19497	17.8
28	608.5324	6762	6.2
29	637.2659	28305	25.9
30	638.2694	8210	7.5