

Mass Spectrum List Report

Analysis Info

Analysis Name D:\Data\ggc\24-121834_P1-B-3_01_9881.d
 Method lc-ms directos tunelow261224 apci.m
 Sample Name 24-121834
 Comment AR30B
 Sv: MeOH + HCOOH
 Manuela García


Acquisition Date 12/26/2024 3:26:44 PM

Operator EB - MV

Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	APCI	Ion Polarity	Positive	Set Nebulizer	1.6 Bar
Focus	Not active	Set Capillary	4500 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	8.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

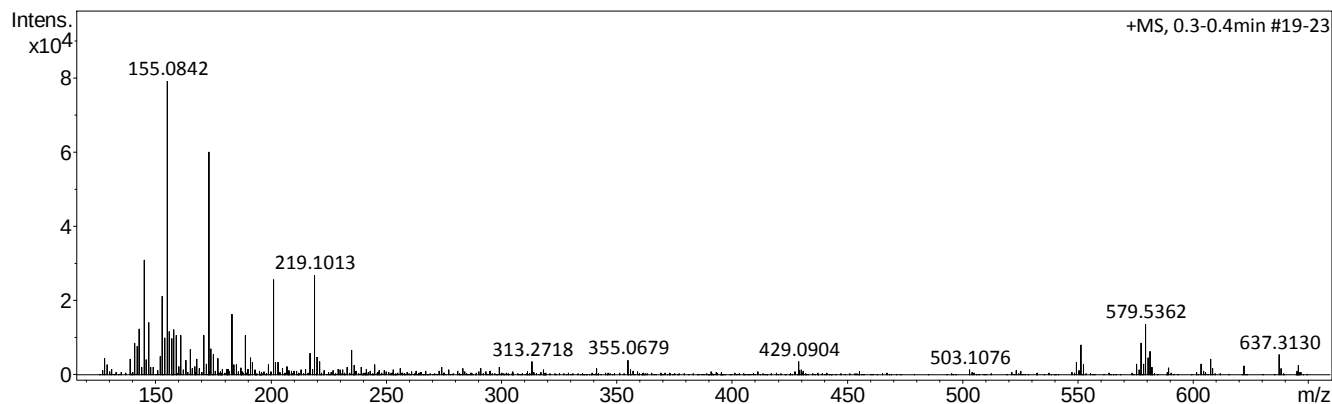

#	m/z	I	I %
1	141.0680	8698	11.0
2	142.0749	7729	9.8
3	143.0835	12405	15.7
4	145.0924	31017	39.3
5	147.0829	14102	17.9
6	152.0606	5117	6.5
7	153.0682	21231	26.9
8	154.0745	10023	12.7
9	155.0842	78939	100.0
10	156.0875	11768	14.9
11	157.0912	9900	12.5
12	158.0743	12272	15.5
13	159.0789	10628	13.5
14	161.0903	10616	13.4
15	165.0725	6869	8.7
16	171.0812	10670	13.5
17	173.0944	60000	76.0
18	174.0967	7087	9.0
19	175.0927	5512	7.0
20	183.0804	16431	20.8
21	189.0912	10689	13.5
22	201.0902	25717	32.6
23	217.0906	5834	7.4
24	219.1013	26829	34.0
25	235.0988	6772	8.6
26	551.5028	8052	10.2
27	577.5197	8644	11.0
28	579.5362	13666	17.3
29	581.2486	6424	8.1
30	637.3130	5626	7.1