

Mass Spectrum List Report

Analysis Info

Analysis Name D:\Data\ggc\24-121835_P1-B-4_01_9882.d
 Method lc-ms directos tunelow261224 apci.m
 Sample Name 24-121835
 Comment GF-C9b
 Sv: MeOH + HCOOH
 Manuela García


Acquisition Date 12/26/2024 3:31:52 PM

Operator EB - MV

Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	APCI	Ion Polarity	Positive	Set Nebulizer	1.6 Bar
Focus	Not active	Set Capillary	4500 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	8.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

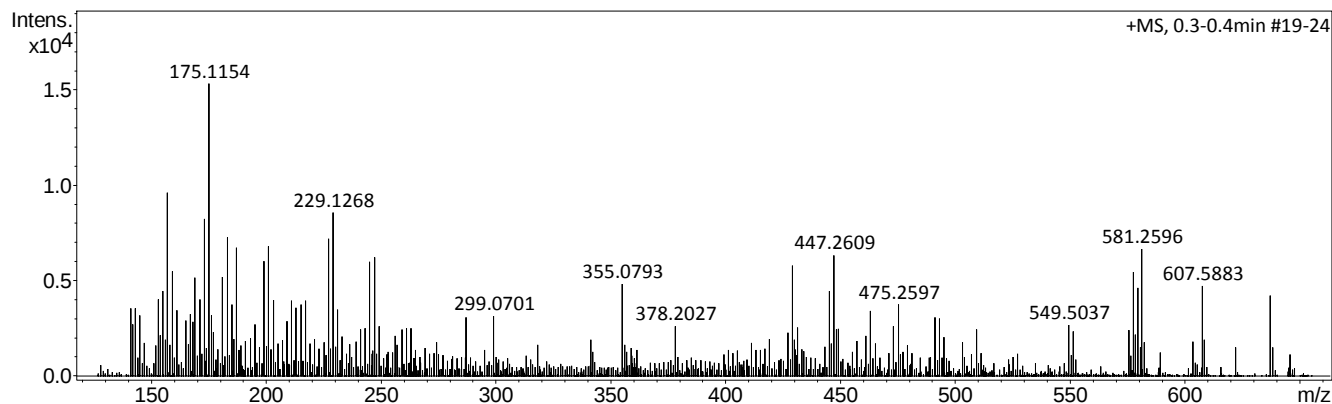

#	m/z	I	I %
1	153.0723	4028	26.4
2	155.0882	4431	29.0
3	157.1024	9588	62.7
4	159.1106	5480	35.9
5	169.1013	5136	33.6
6	171.1111	4009	26.2
7	173.1022	8218	53.8
8	175.1154	15282	100.0
9	181.1033	5190	34.0
10	183.1171	7256	47.5
11	187.1152	6714	43.9
12	199.1169	6007	39.3
13	201.1286	6774	44.3
14	203.1188	3968	26.0
15	211.1175	3937	25.8
16	217.1236	3942	25.8
17	227.1127	7190	47.1
18	229.1268	8553	56.0
19	245.1255	5978	39.1
20	247.1384	6223	40.7
21	355.0793	4800	31.4
22	429.1001	4484	29.3
23	429.2539	5799	37.9
24	445.2514	4448	29.1
25	447.2609	6311	41.3
26	577.5360	5436	35.6
27	579.5502	4624	30.3
28	581.2596	6634	43.4
29	607.5883	4699	30.7
30	637.3239	4230	27.7