

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-060523_P1-F-8_01_9283.d
 Method lc_qtof_directospos.m
 Sample Name 24-060523
 Comment MGP4084a
 Sv: MeOH + HCOOH
 Mariana Pizzio

Acquisition Date 6/12/2024 12:38:43 PM

Operator ELB
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

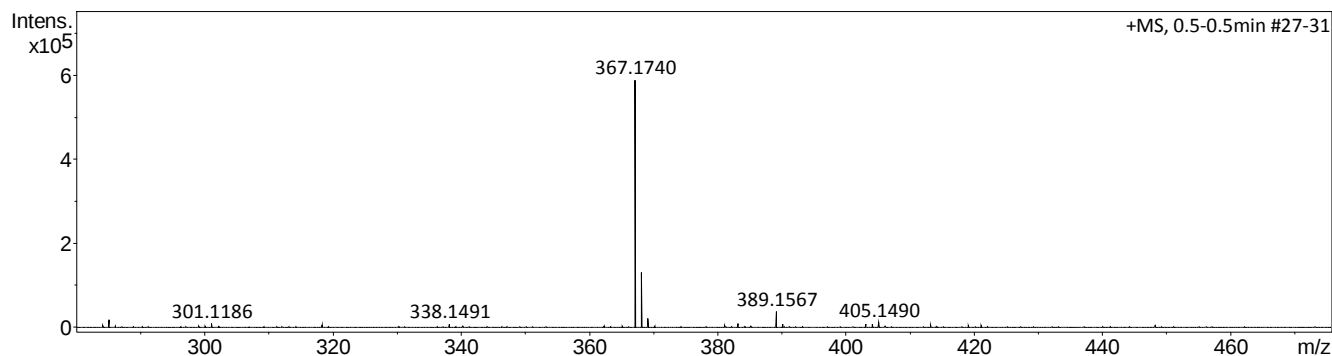

#	m/z	I	I %
1	192.1433	5091	0.9
2	229.1475	3685	0.6
3	251.1300	18652	3.2
4	274.2784	7265	1.2
5	284.1345	5008	0.9
6	285.0952	17802	3.0
7	301.1186	8642	1.5
8	318.3077	6681	1.1
9	338.1491	7865	1.3
10	340.2888	3584	0.6
11	365.1578	3462	0.6
12	367.1740	586970	100.0
13	368.1760	130031	22.2
14	369.1790	21972	3.7
15	381.1532	4430	0.8
16	383.1724	8511	1.5
17	389.1567	37264	6.3
18	390.1573	8299	1.4
19	403.1377	6959	1.2
20	404.1990	7611	1.3
21	405.1490	11730	2.0
22	413.2765	6447	1.1
23	419.1552	5259	0.9
24	421.1484	4691	0.8
25	448.2653	4152	0.7
26	480.2630	4146	0.7
27	539.1894	4362	0.7
28	674.2264	6770	1.2
29	755.3245	9025	1.5
30	756.3220	4160	0.7