

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\24-060524_P1-F-9_01_9284.d
 Method lc_qtof_directospos.m
 Sample Name 24-060524
 Comment MJR2024-7
 Sv: MeOH + HCOOH
 Martín J. Riveira

Acquisition Date 6/12/2024 12:43:47 PM

Operator ELB
 Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

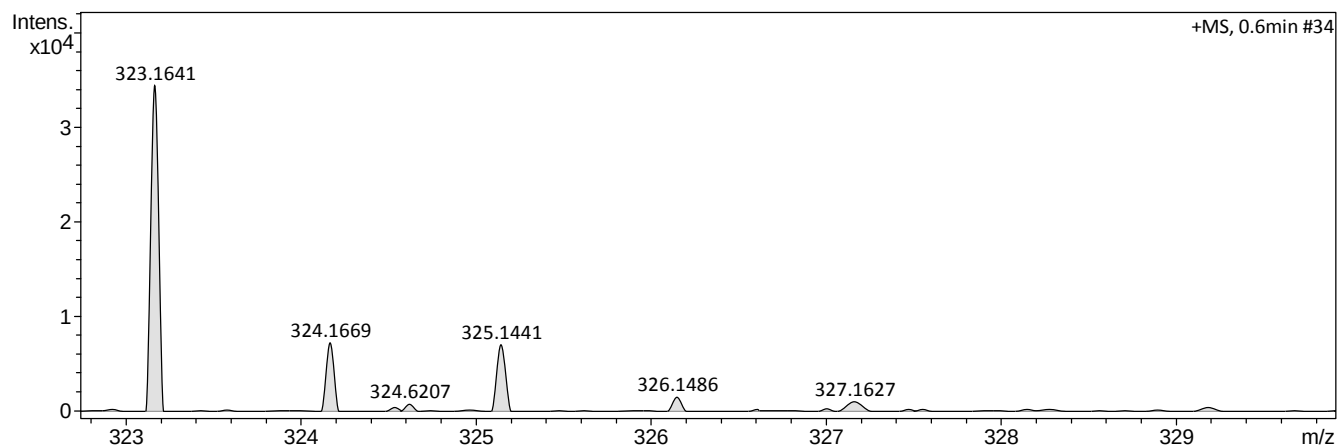

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-060524_P1-F-9_01_9284.d
 Method lc_qtof_directospos.m
 Sample Name 24-060524
 Comment MJR2024-7
 Sv: MeOH + HCOOH
 Martín J. Riveira

Acquisition Date 6/12/2024 12:43:47 PM

Operator ELB
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

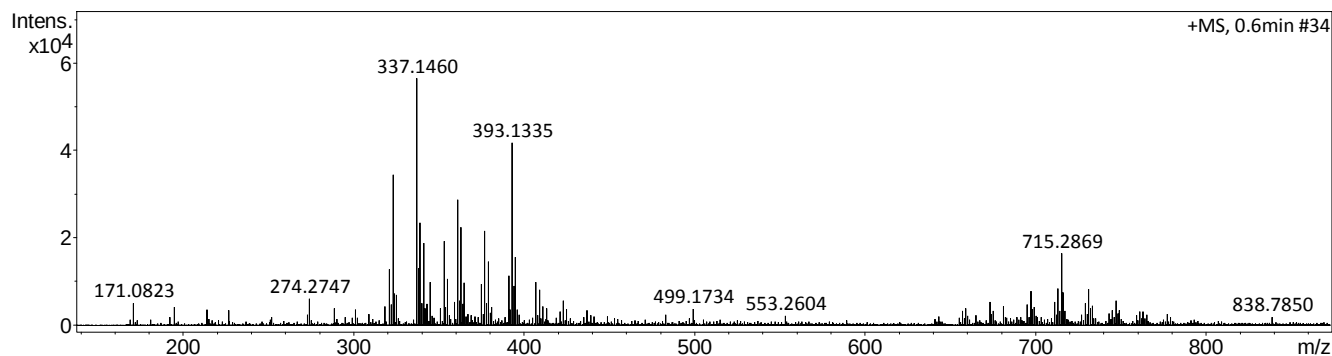

#	m/z	I	I %
1	274.2747	6080	10.8
2	321.1490	12779	22.7
3	323.1641	34381	61.0
4	324.1669	7204	12.8
5	325.1441	6988	12.4
6	337.1460	56377	100.0
7	338.1502	13005	23.1
8	339.1602	23464	41.6
9	341.1424	18683	33.1
10	345.1482	9809	17.4
11	353.1410	19185	34.0
12	355.1545	10584	18.8
13	361.1428	28649	50.8
14	362.1446	5628	10.0
15	363.1244	22359	39.7
16	365.1079	9646	17.1
17	375.1215	9425	16.7
18	377.1344	21473	38.1
19	379.1362	14467	25.7
20	391.1388	11282	20.0
21	393.1335	41646	73.9
22	394.1384	9026	16.0
23	395.1411	15472	27.4
24	407.1359	9809	17.4
25	409.1274	8088	14.3
26	697.2766	7814	13.9
27	713.2704	8371	14.8
28	715.2869	16367	29.0
29	716.2970	7537	13.4
30	731.2800	8233	14.6