

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\BP129B_P1-C-4_01_8429.d
 Method lc_qtof_directospos.m
 Sample Name BP129B
 Comment Sv: MeOH + HCOOH
 Sonogo

Acquisition Date 12/28/2023 12:30:17 PM

Operator ELB
 Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

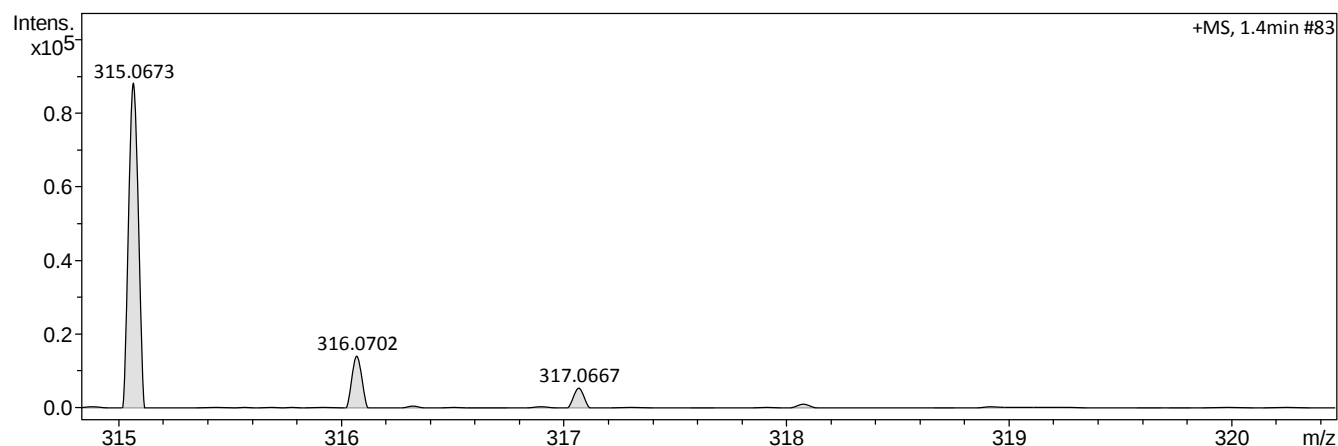

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
315.0673	1	C15H16NaO4S	315.0662	-3.7	7.8	1	63.77	7.5	even	ok