

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\BP131_P1-C-9_01_8434.d
 Method lc_qtof_directospos.m
 Sample Name BP131
 Comment Sv: MeOH + HCOOH
 Sonogo

Acquisition Date 12/28/2023 12:55:36 PM

Operator ELB
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

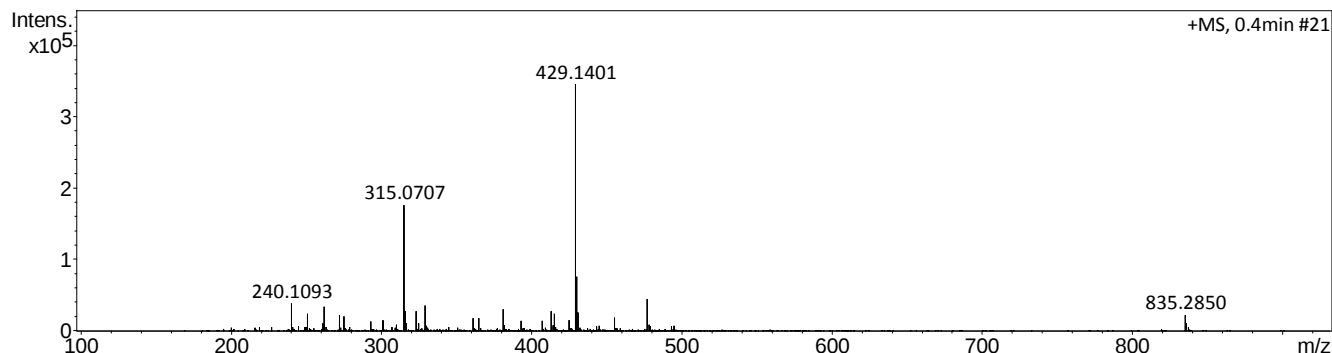

#	m/z	I	I %
1	240.1093	38324	11.1
2	251.0210	23810	6.9
3	261.1073	10985	3.2
4	262.0908	34172	9.9
5	272.2044	22358	6.5
6	275.1298	20371	5.9
7	293.0942	9889	2.9
8	293.1700	13532	3.9
9	301.1038	15346	4.5
10	315.0707	175974	51.0
11	316.0729	27329	7.9
12	317.0716	10424	3.0
13	323.0829	27223	7.9
14	325.1438	11081	3.2
15	329.1756	35294	10.2
16	361.0418	17657	5.1
17	365.1748	17514	5.1
18	381.1723	30435	8.8
19	393.3005	13843	4.0
20	407.1548	13921	4.0
21	413.2712	27322	7.9
22	415.1216	24077	7.0
23	424.9835	15185	4.4
24	429.1401	344752	100.0
25	430.1412	75790	22.0
26	431.1367	26038	7.6
27	455.1466	19037	5.5
28	477.1307	44320	12.9
29	835.2850	22110	6.4
30	836.2864	10507	3.0