

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\BP132_P1-C-8_01_8433.d
 Method lc_qtof_directospos.m
 Sample Name BP132
 Comment Sv: MeOH + HCOOH
 Sonogo

Acquisition Date 12/28/2023 12:50:33 PM

Operator ELB
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

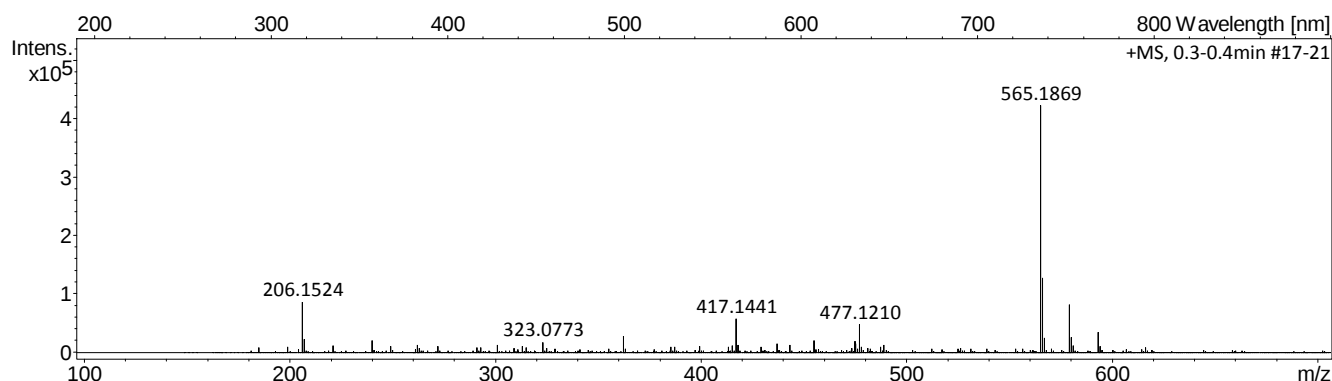

#	m/z	I	I %
1	206.1524	86107	20.4
2	207.0436	22566	5.4
3	207.1555	12959	3.1
4	221.0592	11375	2.7
5	240.1050	19933	4.7
6	262.0860	12910	3.1
7	272.2003	10735	2.5
8	301.0953	12698	3.0
9	313.0840	10518	2.5
10	323.0773	17295	4.1
11	362.2383	27430	6.5
12	399.3046	10400	2.5
13	415.1202	11902	2.8
14	417.1441	57124	13.6
15	418.1449	12657	3.0
16	437.1180	14610	3.5
17	443.3292	12240	2.9
18	455.1366	20178	4.8
19	475.1413	18748	4.4
20	475.3217	14950	3.5
21	477.1210	47883	11.4
22	489.1255	12700	3.0
23	565.1869	421470	100.0
24	566.1900	127129	30.2
25	567.1887	25058	5.9
26	579.1652	81204	19.3
27	580.1683	25256	6.0
28	581.1673	12013	2.9
29	593.1441	33915	8.0
30	594.1469	10496	2.5