

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\BP139C_P1-C-5_01_8430.d
 Method lc_qtof_directospos.m
 Sample Name BP139C
 Comment Sv: MeOH + HCOOH
 Sonogo

Acquisition Date 12/28/2023 12:35:20 PM

Operator ELB
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

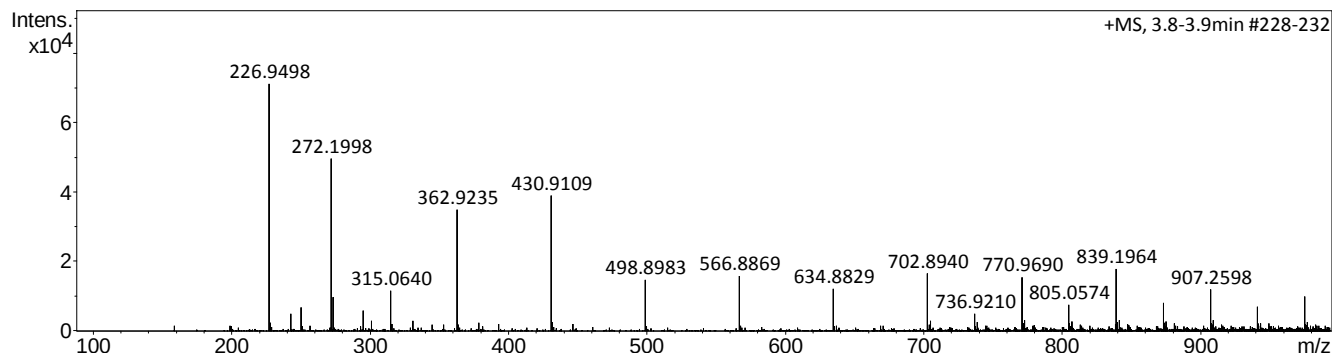

#	m/z	I	I %
1	226.9498	70984	100.0
2	242.9255	4879	6.9
3	250.1421	6791	9.6
4	272.1998	49520	69.8
5	273.2026	9673	13.6
6	294.9368	5817	8.2
7	301.1392	2974	4.2
8	315.0640	11587	16.3
9	331.0355	2878	4.1
10	362.9235	34844	49.1
11	430.9109	38960	54.9
12	431.9125	2609	3.7
13	498.8983	14647	20.6
14	566.8869	15805	22.3
15	634.8829	12170	17.1
16	702.8940	16559	23.3
17	704.8872	2882	4.1
18	736.9210	4892	6.9
19	770.9690	15415	21.7
20	772.9639	3197	4.5
21	805.0574	7447	10.5
22	807.0515	2739	3.9
23	839.1964	17864	25.2
24	841.1761	3176	4.5
25	873.2221	8068	11.4
26	875.2155	2714	3.8
27	907.2598	11870	16.7
28	909.2547	3095	4.4
29	941.3053	7032	9.9
30	975.3480	9902	13.9