

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\BP143_P1-D-2_01_8436.d
 Method lc_qtof_directospos.m
 Sample Name BP143
 Comment Sv: MeOH + HCOOH
 Sonogo

Acquisition Date 12/28/2023 1:05:43 PM

Operator ELB
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

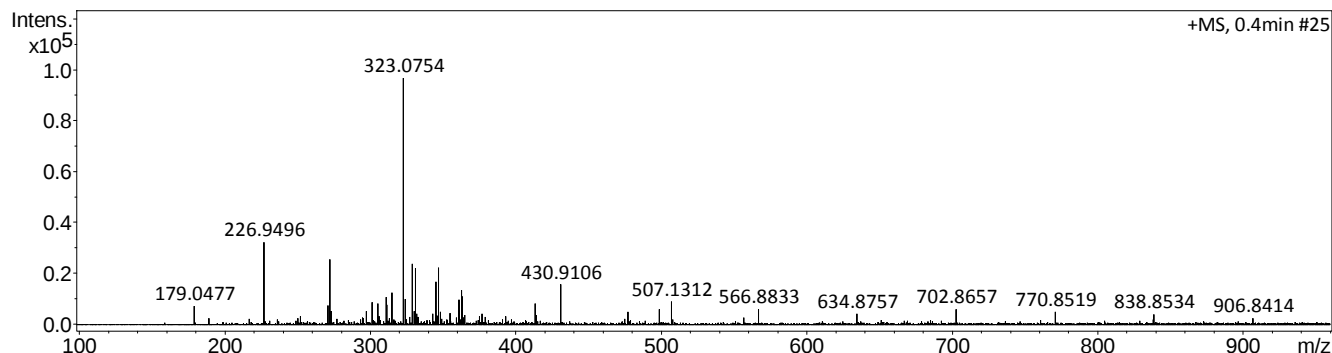

#	m/z	I	I %
1	179.0477	7135	7.4
2	226.9496	32231	33.4
3	270.9765	7400	7.7
4	272.1968	25519	26.5
5	273.1995	5221	5.4
6	297.2369	5049	5.2
7	301.1106	8675	9.0
8	305.1958	8222	8.5
9	311.0757	10723	11.1
10	311.2518	7737	8.0
11	315.0654	12406	12.9
12	323.0754	96437	100.0
13	324.0782	10011	10.4
14	329.1677	23701	24.6
15	330.1710	5067	5.3
16	331.1806	21902	22.7
17	345.1633	16640	17.3
18	347.1761	22144	23.0
19	348.1814	4806	5.0
20	361.1668	9693	10.1
21	362.9227	13431	13.9
22	363.1728	10981	11.4
23	413.2815	8210	8.5
24	430.9106	15689	16.3
25	477.1190	4924	5.1
26	498.8974	5922	6.1
27	507.1312	8910	9.2
28	566.8833	6001	6.2
29	702.8657	5853	6.1
30	770.8519	4782	5.0