

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-112201_P1-C-3_01_9773.d
 Method lc ms directos_241016neg.m
 Sample Name 24-112201
 Comment A2-DT1
 Sv: DCM + MeOH
 Mario Salazar - UNR CONICET

Acquisition Date 11/25/2024 1:45:30 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Negative	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	3500 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

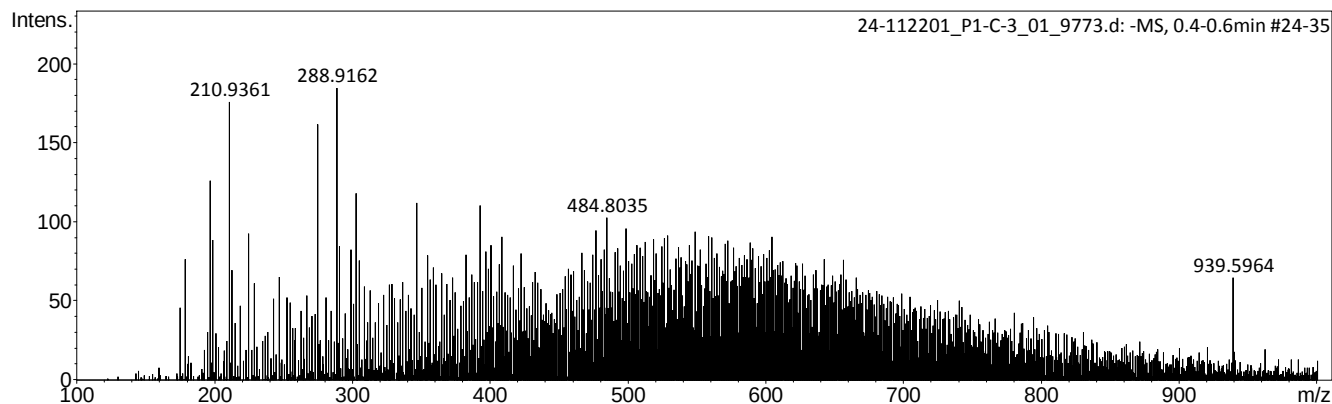

#	m/z	I	I %
1	196.9232	126	68.4
2	198.9169	88	47.9
3	210.9361	175	95.1
4	224.9514	92	50.1
5	274.8986	161	87.4
6	288.9162	184	100.0
7	290.8982	84	45.7
8	302.9244	118	64.0
9	346.8534	112	60.7
10	392.8517	110	59.8
11	400.8440	85	46.1
12	408.8377	90	49.0
13	476.8085	94	51.2
14	484.8035	103	55.6
15	498.7917	96	51.9
16	506.7911	85	46.2
17	512.7869	87	47.2
18	518.7765	89	48.1
19	524.7836	84	45.7
20	526.7768	90	48.6
21	528.7811	91	49.5
22	536.7759	84	45.5
23	544.7692	85	46.1
24	548.7616	94	50.8
25	558.7591	91	49.3
26	560.7706	90	48.8
27	570.7496	86	46.7
28	572.7656	88	47.7
29	588.7524	87	47.1
30	604.7418	90	49.0