

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-112201_P1-C-3_01_9768.d
 Method lc_ms directos tunelow300924.m
 Sample Name 24-112201
 Comment A2-DT1
 Sv: DCM + MeOH + HCOOH
 Mario Salazar - UNR CONICET

Acquisition Date 11/25/2024 12:30:32 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

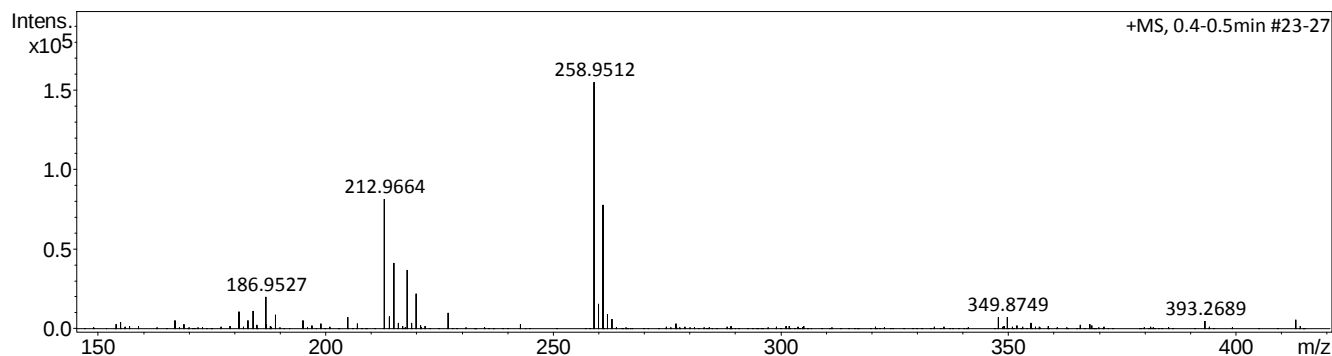

#	m/z	I	I %
1	154.9815	3917	2.5
2	166.8939	5187	3.4
3	166.9803	3956	2.6
4	180.9951	10709	6.9
5	182.9944	5335	3.4
6	184.0608	11464	7.4
7	186.9527	19962	12.9
8	188.9492	9051	5.8
9	195.0141	5174	3.3
10	204.9614	7363	4.8
11	206.9597	3379	2.2
12	212.9664	81351	52.6
13	213.9686	7838	5.1
14	214.9641	41212	26.6
15	215.9666	3664	2.4
16	217.9150	36855	23.8
17	218.9175	3663	2.4
18	219.9126	22081	14.3
19	226.9386	9967	6.4
20	258.9512	154765	100.0
21	259.9537	15821	10.2
22	260.9495	77822	50.3
23	261.9518	9338	6.0
24	262.9457	6234	4.0
25	347.8785	7231	4.7
26	349.8749	7265	4.7
27	355.0480	3537	2.3
28	393.2689	4758	3.1
29	413.2431	5742	3.7
30	685.3942	3970	2.6