

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\24-112202_P1-C-1_01_9766.d
 Method lc_ms directos tunelow300924.m
 Sample Name 24-112202
 Comment AME1
 Sv: MeOH + HCOOH
 Mario Salazar - UNR CONICET

Acquisition Date 11/25/2024 10:44:56 AM

Operator EB - MV
 Instrument micrOTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

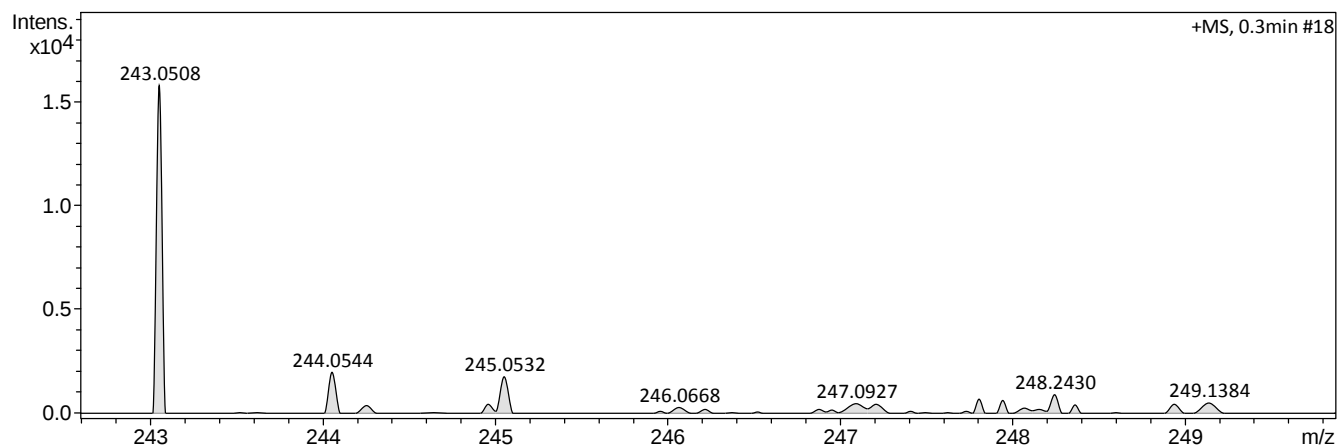

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
243.0508	1	C11H15O2S2	243.0508	0.2	10.2	1	100.00	4.5	even	ok