

Mass Spectrum List Report

Analysis Info

Analysis Name D:\Data\ggc\24-112203_P1-C-4_01_9774.d
 Method lc ms directos_241016neg.m
 Sample Name 24-112203
 Comment AME2
 Sv: MeOH
 Mario Salazar - UNR CONICET


Acquisition Date 11/25/2024 1:53:56 PM

Operator EB - MV

Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Negative	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	3500 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

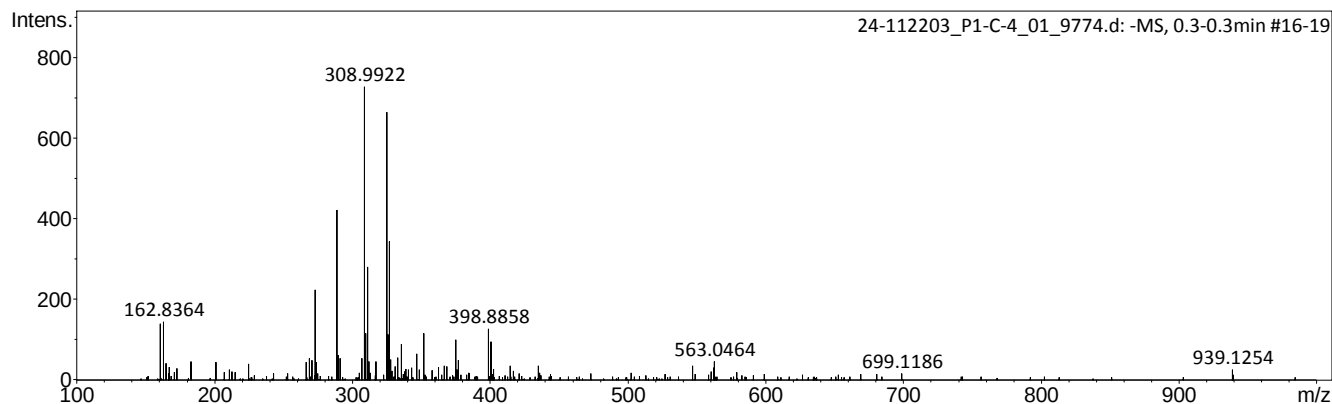

#	m/z	I	I %
1	160.8387	140	19.2
2	162.8364	143	19.7
3	183.0090	46	6.3
4	201.0147	44	6.1
5	268.7917	53	7.3
6	270.7949	49	6.7
7	273.0171	224	30.8
8	274.0238	44	6.0
9	289.0108	421	57.9
10	290.0138	61	8.4
11	291.0065	53	7.3
12	306.9847	53	7.3
13	308.9922	727	100.0
14	309.9934	115	15.8
15	310.9906	281	38.6
16	311.9908	45	6.2
17	317.0288	45	6.2
18	324.9861	663	91.2
19	325.9897	112	15.5
20	326.9815	343	47.2
21	327.9850	50	6.9
22	333.1198	55	7.5
23	336.0118	88	12.1
24	346.9446	64	8.8
25	352.0051	115	15.9
26	375.0582	99	13.6
27	377.0658	49	6.7
28	398.8858	126	17.4
29	400.8822	95	13.1
30	563.0464	46	6.3