

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-112203_P1-C-4_01_9769.d
 Method lc_ms directos tunelow300924.m
 Sample Name 24-112203
 Comment AME2
 Sv: MeOH + HCOOH
 Mario Salazar - UNR CONICET

Acquisition Date 11/25/2024 12:35:39 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

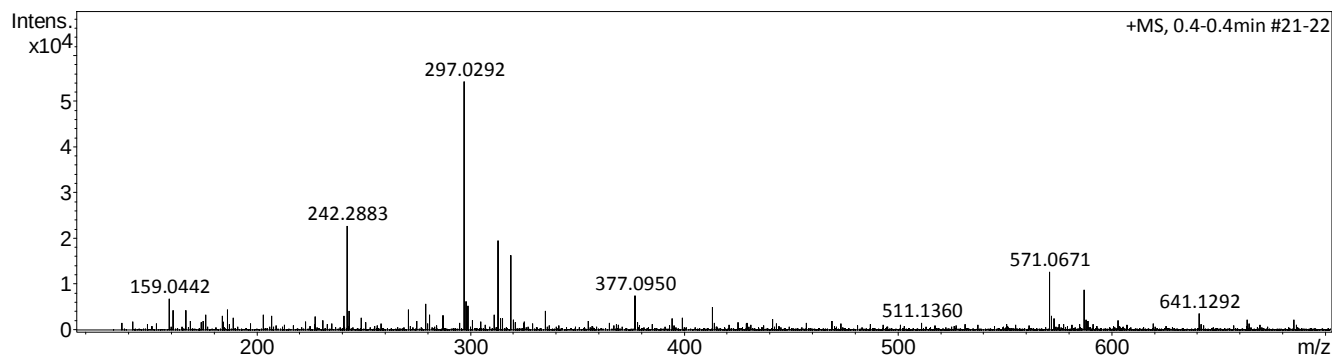

#	m/z	I	I %
1	159.0442	6788	12.5
2	160.9733	4356	8.0
3	167.0212	4349	8.0
4	176.1462	3264	6.0
5	184.0767	2967	5.5
6	186.2253	4437	8.2
7	189.0045	2598	4.8
8	203.0253	3285	6.1
9	207.0128	3025	5.6
10	227.2071	2839	5.2
11	240.9711	3042	5.6
12	242.2883	22710	41.9
13	243.2946	4135	7.6
14	271.1023	4398	8.1
15	279.0185	5726	10.6
16	281.0367	3335	6.2
17	287.1005	3143	5.8
18	297.0292	54182	100.0
19	298.0340	6279	11.6
20	299.0280	5262	9.7
21	311.0452	3277	6.0
22	313.0209	19412	35.8
23	319.0117	16298	30.1
24	334.9986	4177	7.7
25	377.0950	7530	13.9
26	413.2784	5029	9.3
27	571.0671	12680	23.4
28	572.0679	3088	5.7
29	587.0606	8689	16.0
30	641.1292	3591	6.6