

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-112204_P1-C-5_01_9775.d
 Method lc ms directos_241016neg.m
 Sample Name 24-112204
 Comment AME3
 Sv: MeOH
 Mario Salazar - UNR CONICET

Acquisition Date 11/26/2024 10:40:36 AM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Negative	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	3500 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

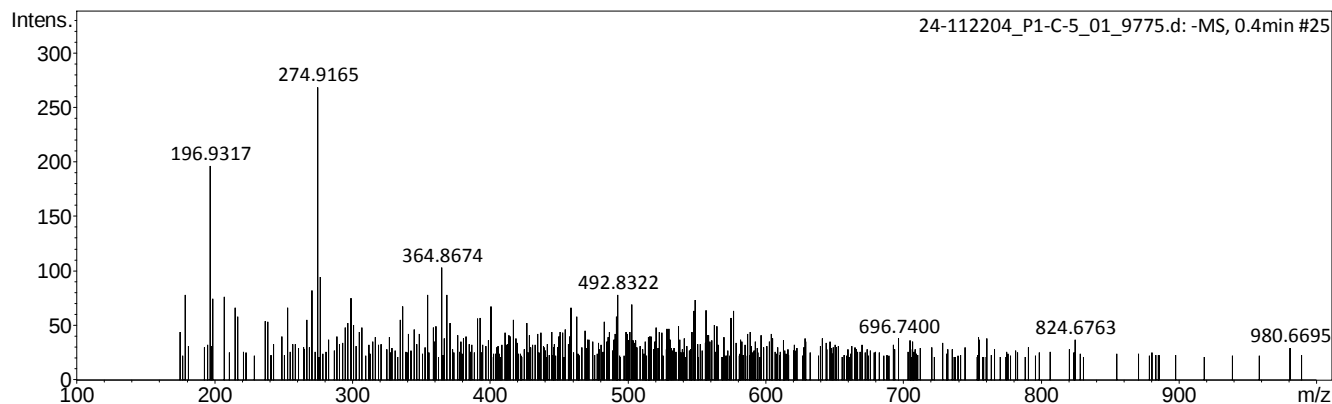

#	m/z	I	I %
1	178.9176	78	29.1
2	196.9317	196	73.1
3	198.9249	74	27.6
4	206.9920	76	28.4
5	214.9389	66	24.6
6	216.9274	58	21.6
7	252.9033	66	24.6
8	266.8987	55	20.5
9	270.9036	82	30.6
10	274.9165	268	100.0
11	276.9111	94	35.1
12	298.9044	75	28.0
13	334.8957	55	20.5
14	336.8895	67	25.0
15	354.9107	78	29.1
16	364.8674	103	38.4
17	368.8890	78	29.1
18	390.8639	56	20.9
19	392.8900	57	21.3
20	400.8867	67	25.0
21	458.8440	66	24.6
22	462.8011	58	21.6
23	491.7953	58	21.6
24	492.8322	78	29.1
25	502.8325	69	25.7
26	547.8438	63	23.5
27	548.8246	73	27.2
28	556.8181	64	23.9
29	574.7900	57	21.3
30	576.8090	63	23.5