

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-112204_P1-C-5_01_9770.d
 Method lc_ms directos tunelow300924.m
 Sample Name 24-112204
 Comment AME3
 Sv: MeOH + HCOOH
 Mario Salazar - UNR CONICET

Acquisition Date 11/25/2024 12:40:48 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

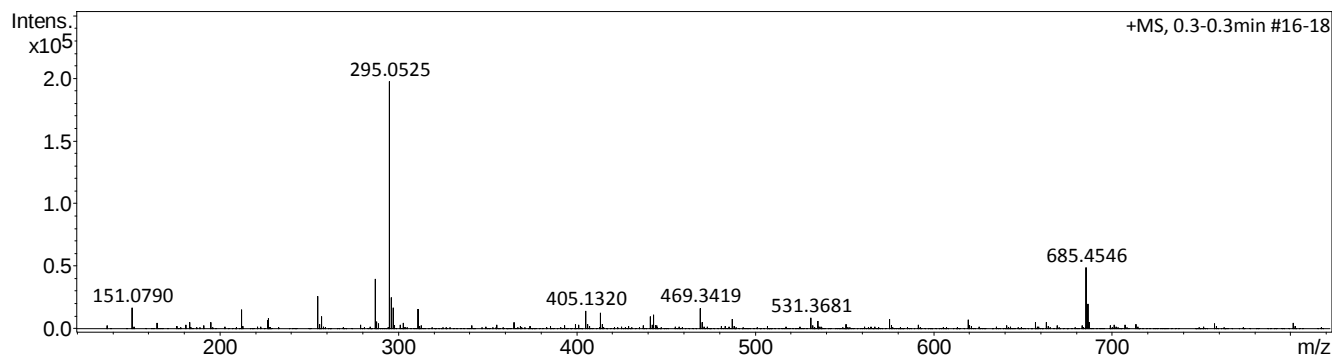

#	m/z	I	I %
1	151.0790	17111	8.7
2	183.0507	5283	2.7
3	212.1226	15165	7.7
4	227.0362	6765	3.4
5	227.2074	7989	4.1
6	255.0580	26292	13.3
7	257.0706	9709	4.9
8	287.0252	39680	20.1
9	288.0271	5476	2.8
10	295.0525	197157	100.0
11	296.0543	24884	12.6
12	297.0483	17069	8.7
13	311.0459	15670	7.9
14	365.1184	5273	2.7
15	405.1320	14147	7.2
16	413.2787	13031	6.6
17	441.3067	9725	4.9
18	443.1090	11271	5.7
19	443.3102	5504	2.8
20	469.3419	16383	8.3
21	487.3415	7786	3.9
22	531.3681	8572	4.3
23	535.1241	6426	3.3
24	575.3949	7809	4.0
25	619.4225	7004	3.6
26	663.4468	5284	2.7
27	685.4546	48927	24.8
28	686.4562	20086	10.2
29	687.4607	5324	2.7
30	957.5164	7428	3.8