

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\24-112205_P1-C-6_01_9776.d
 Method lc ms directos_241016neg.m
 Sample Name 24-112205
 Comment A6-EDT
 Sv: MeOH + HCOOH
 Mario Salazar - UNR CONICET

Acquisition Date 11/26/2024 10:45:43 AM

Operator EB - MV
 Instrument micrOTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Negative	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	3500 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

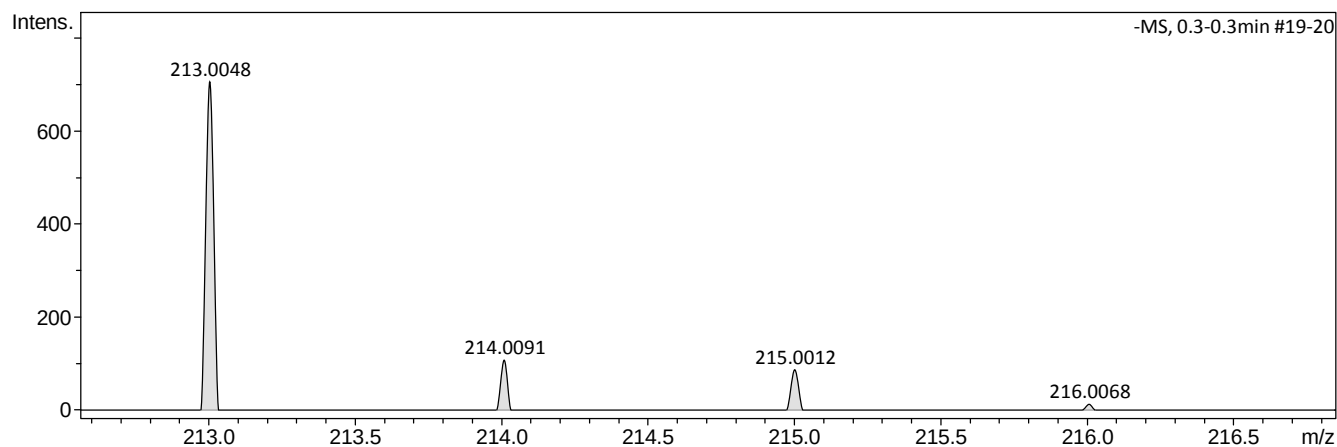

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
213.0048	1	C9H9O2S2	213.0049	0.7	22.5	1	100.00	5.5	even	ok