

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-112205_P1-C-6_01_9776.d
 Method lc ms directos_241016neg.m
 Sample Name 24-112205
 Comment A6-EDT
 Sv: MeOH + HCOOH
 Mario Salazar - UNR CONICET

Acquisition Date 11/26/2024 10:45:43 AM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Negative	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	3500 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

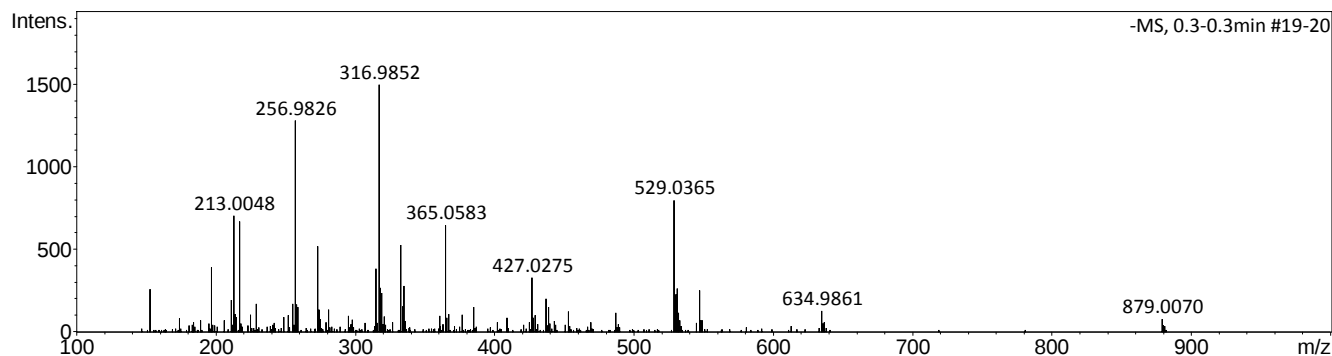

#	m/z	I	I %
1	153.0042	260	17.4
2	196.9756	391	26.1
3	210.9937	194	12.9
4	213.0048	705	47.1
5	217.0758	669	44.7
6	228.9976	169	11.3
7	255.0134	170	11.4
8	256.9826	1281	85.6
9	257.9835	165	11.0
10	258.9798	153	10.2
11	273.0267	517	34.5
12	274.0308	133	8.9
13	281.0001	136	9.1
14	315.0192	384	25.7
15	316.9852	1496	100.0
16	317.9940	265	17.7
17	318.9802	237	15.9
18	333.0316	526	35.2
19	334.0314	155	10.3
20	335.0449	277	18.5
21	365.0583	644	43.0
22	384.9761	149	10.0
23	427.0275	327	21.9
24	437.0057	199	13.3
25	439.0124	149	10.0
26	529.0365	795	53.1
27	530.0399	227	15.2
28	531.0118	264	17.6
29	547.0378	252	16.9
30	634.9861	129	8.6