

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-112205_P1-C-6_01_9771.d
 Method lc_ms directos tunelow300924.m
 Sample Name 24-112205
 Comment A6-EDT
 Sv: MeOH + HCOOH
 Mario Salazar - UNR CONICET

Acquisition Date 11/25/2024 12:45:56 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

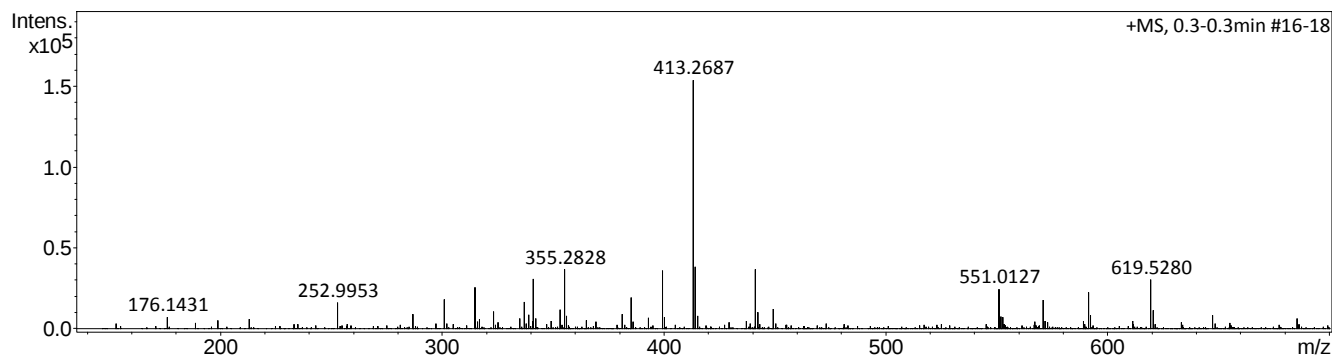

#	m/z	I	I %
1	252.9953	16411	10.7
2	286.9829	8985	5.9
3	301.1397	18027	11.8
4	315.0151	25633	16.7
5	323.2122	10715	7.0
6	336.9974	16501	10.8
7	339.0095	8572	5.6
8	341.2655	30904	20.2
9	353.2668	12013	7.8
10	355.2828	36834	24.0
11	356.2875	7887	5.1
12	381.2963	9014	5.9
13	385.2930	19276	12.6
14	399.3064	36126	23.6
15	413.2687	153316	100.0
16	414.2716	38146	24.9
17	415.2719	8078	5.3
18	441.2992	36878	24.1
19	442.2985	10194	6.6
20	449.3634	12470	8.1
21	551.0127	24345	15.9
22	552.0137	7585	4.9
23	571.0339	17964	11.7
24	591.4977	22445	14.6
25	592.5035	8245	5.4
26	619.5280	30343	19.8
27	620.5306	11637	7.6
28	647.5623	8293	5.4
29	853.7270	7365	4.8
30	881.7534	8484	5.5