

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-112206_P1-C-2_01_9767.d
 Method lc_ms directos tunelow300924.m
 Sample Name 24-112206
 Comment PFC1 (218-MAI-2)
 Sv: MeOH + HCOOH
 Mario Salazar - UNR CONICET

Acquisition Date 11/25/2024 11:43:14 AM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

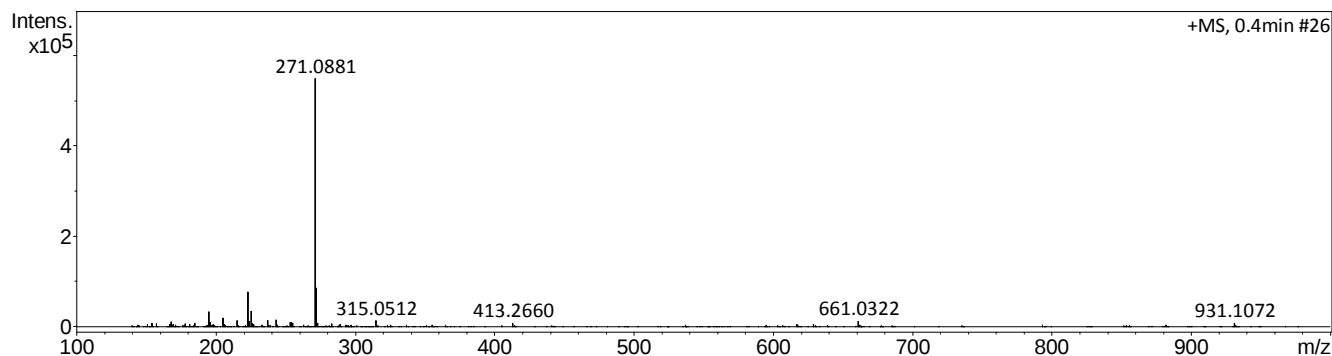

#	m/z	I	I %
1	151.0246	6281	1.1
2	154.0318	8754	1.6
3	157.0753	6724	1.2
4	168.0637	11134	2.0
5	178.0635	6416	1.2
6	181.0744	5953	1.1
7	185.0699	8082	1.5
8	195.0898	33321	6.1
9	196.0786	10416	1.9
10	205.0753	19830	3.6
11	215.0965	13672	2.5
12	223.0864	78001	14.2
13	224.0853	12449	2.3
14	225.0820	35478	6.5
15	226.0761	6923	1.3
16	237.1019	14721	2.7
17	243.0911	15216	2.8
18	253.0959	10448	1.9
19	254.0646	10201	1.9
20	255.0876	7776	1.4
21	271.0881	547957	100.0
22	272.0903	85829	15.7
23	273.0931	8096	1.5
24	283.0900	6367	1.2
25	289.0797	6111	1.1
26	315.0512	14752	2.7
27	413.2660	8477	1.5
28	629.0918	5870	1.1
29	661.0322	12790	2.3
30	931.1072	7757	1.4