

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-112503_P1-E-4_01_9798.d
 Method lc_ms directos tunelow300924.m
 Sample Name 24-112503
 Comment PIRF3F4T18
 Sv: DCM + MeOH + HCOOH
 Carlos Solis - UNR

Acquisition Date 12/3/2024 10:13:43 AM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

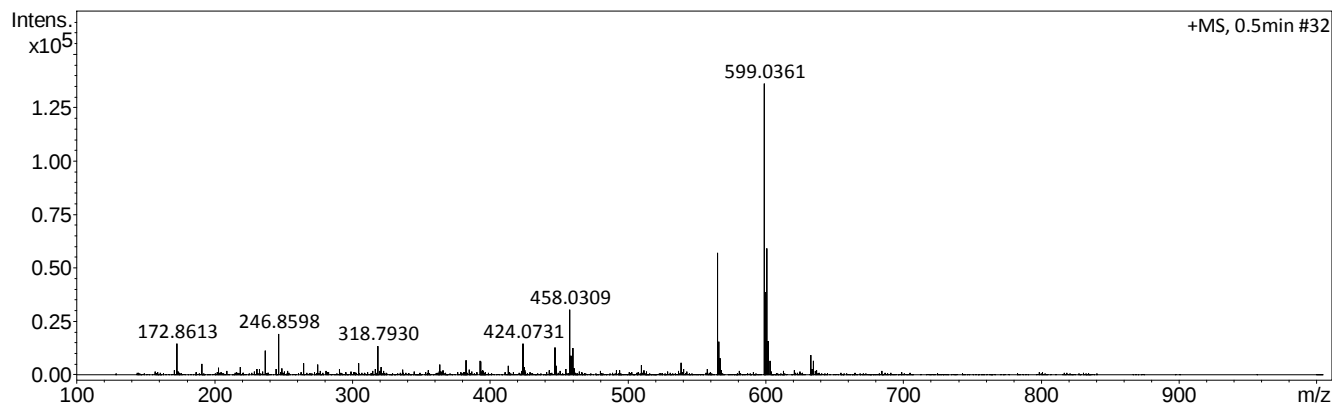

#	m/z	I	I %
1	172.8613	14689	10.8
2	190.8683	5101	3.7
3	236.9039	11558	8.5
4	246.8598	19253	14.1
5	264.8718	5424	4.0
6	274.8054	5018	3.7
7	304.8923	5344	3.9
8	318.7930	13638	10.0
9	363.7881	4948	3.6
10	382.8327	7083	5.2
11	392.7905	6717	4.9
12	393.2963	6437	4.7
13	413.2647	4391	3.2
14	424.0731	14653	10.8
15	447.3442	12951	9.5
16	458.0309	30479	22.4
17	459.0351	9125	6.7
18	460.0298	12706	9.3
19	509.7202	4455	3.3
20	538.7196	5783	4.2
21	565.0727	57009	41.9
22	566.0753	15567	11.4
23	567.0775	7840	5.8
24	599.0361	136104	100.0
25	600.0393	38579	28.3
26	601.0335	59092	43.4
27	602.0371	15800	11.6
28	603.0313	6603	4.9
29	632.9977	9301	6.8
30	635.0063	6650	4.9