

Mass Spectrum List Report

Analysis Info

Analysis Name D:\Data\ggc\24-112504_P1-E-5_01_9792.d
 Method lc_ms directos tunelow300924.m
 Sample Name 24-112504
 Comment PIRF3F4T26A
 Sv: DCM + MeOH + HCOOH
 Carlos Solis - UNR


Acquisition Date 11/28/2024 2:11:05 PM

Operator EB - MV

Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

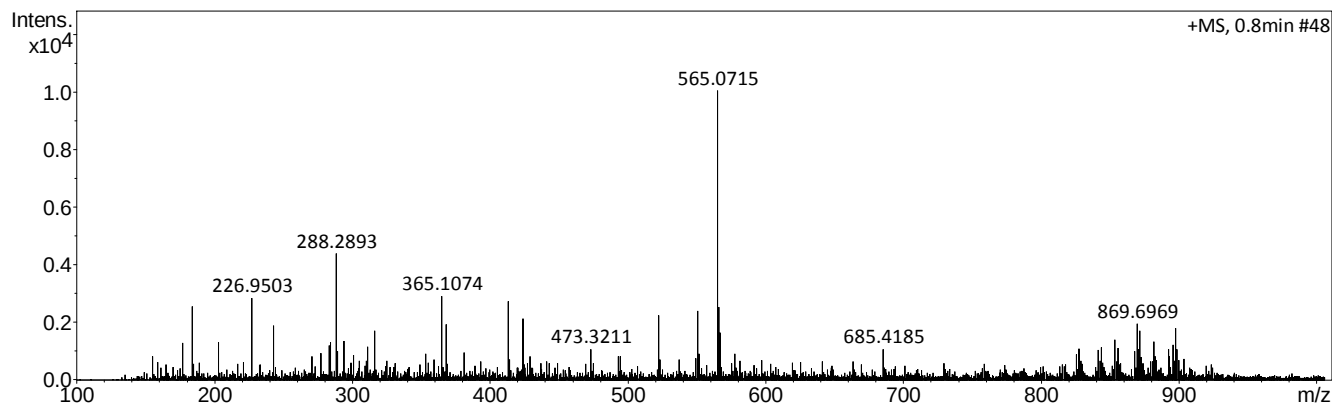

#	m/z	I	I %
1	177.1148	1289	12.8
2	184.0725	2544	25.3
3	203.0520	1312	13.1
4	226.9503	2834	28.2
5	242.9260	1876	18.7
6	283.2617	1196	11.9
7	284.3277	1312	13.1
8	288.2893	4382	43.6
9	294.1285	1353	13.5
10	311.2882	1158	11.5
11	316.3195	1707	17.0
12	365.1074	2908	29.0
13	368.4242	1922	19.1
14	413.2632	2730	27.2
15	424.0690	2117	21.1
16	522.5935	2234	22.3
17	550.6261	2397	23.9
18	565.0715	10039	100.0
19	566.0748	2523	25.1
20	567.0733	1629	16.2
21	827.7054	1081	10.8
22	843.6764	1133	11.3
23	853.7181	1399	13.9
24	855.7205	1097	10.9
25	869.6969	1945	19.4
26	871.7166	1703	17.0
27	881.7402	1333	13.3
28	892.7087	1066	10.6
29	895.7045	1213	12.1
30	897.7278	1783	17.8