

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\24-112504_P1-E-5_01_9792.d
 Method lc_ms directos tunelow300924.m
 Sample Name 24-112504
 Comment PIRF3F4T26A
 Sv: DCM + MeOH + HCOOH
 Carlos Solis - UNR

Acquisition Date 11/28/2024 2:11:05 PM

Operator EB - MV
 Instrument micrOTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

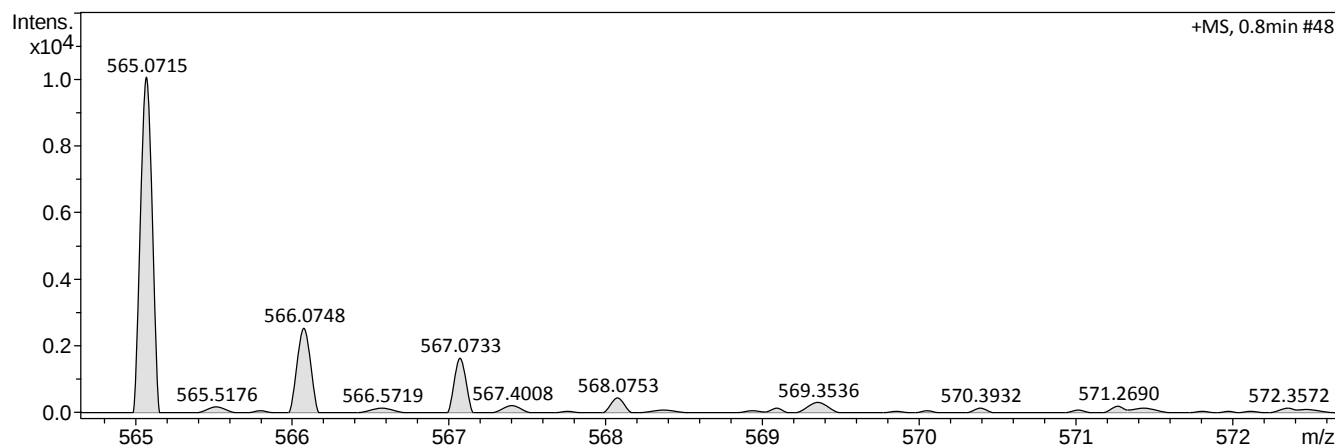

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
565.0715	1	C27H21N2O8S2	565.0734	3.4	31.5	1	100.00	18.5	even	ok