

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\BM26#1_P1-D-2_01_9159.d
 Method lc_qtof_directospos.m
 Sample Name BM26#1
 Comment Sv: MeOH + HCOOH
 Szajnman

Acquisition Date 5/6/2024 3:58:18 PM

Operator ELB
 Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

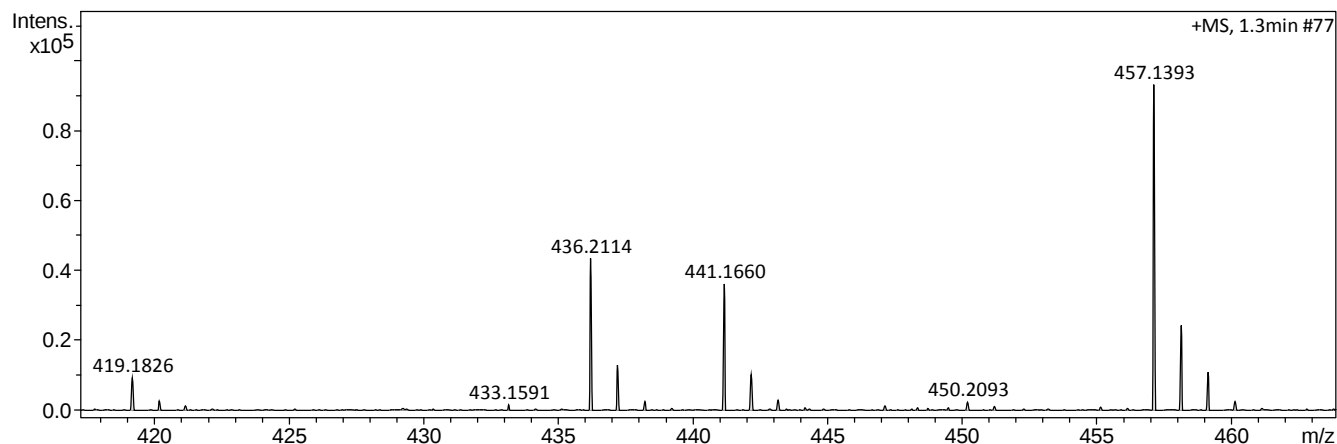

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdB	e ⁻ Conf	N-Rule
419.1826	1	C26H27O5	419.1853	6.4	29.0	1	100.00	13.5	even	ok
436.2114	1	C26H30NO5	436.2118	1.0	5.1	1	100.00	12.5	even	ok
441.1660	1	C26H26NaO5	441.1672	2.8	17.5	1	47.31	13.5	even	ok
457.1393	1	C26H26KO5	457.1412	4.1	13.4	1	100.00	13.5	even	ok