

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\BM80#1bis_P1-B-4_01_9659.d
 Method lc_ms directos tunelow300924.m
 Sample Name BM80#1bis
 Comment Sv: MeOH + HCOOH
 Sergio Szajnman

Acquisition Date 11/8/2024 12:59:45 PM

Operator EB - MV
 Instrument micrOTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

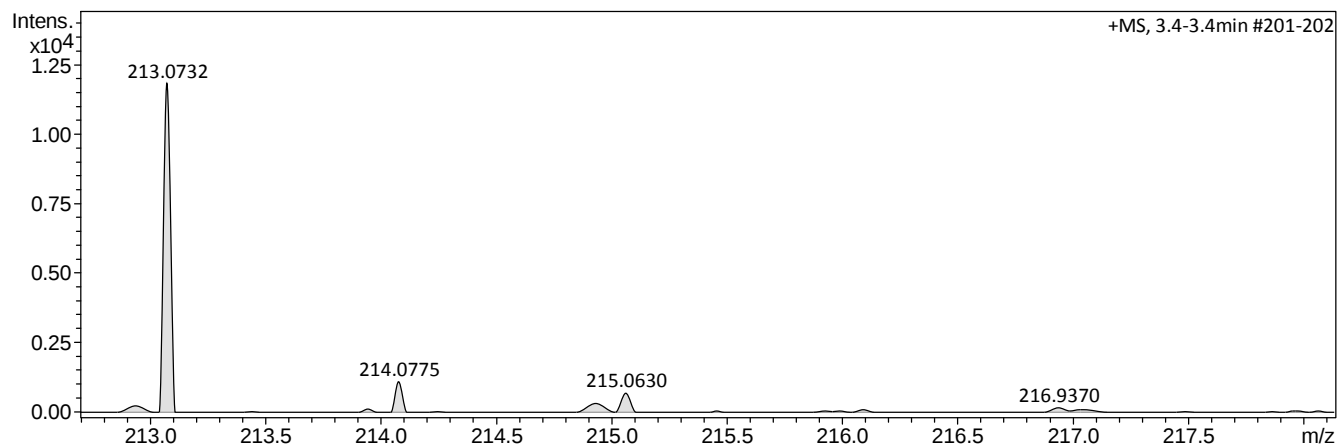

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdB	e ⁻ Conf	N-Rule
213.0732	1	C8H14NaO5	213.0733	0.4	8.0	3	97.58	1.5	even	ok