

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\HG-162_P1-D-3_01_9227.d
 Method lc_qtof_directospos.m
 Sample Name HG-162
 Comment Sv: MeOH + HCOOH
 Szajnman

Acquisition Date 6/6/2024 10:57:16 AM

Operator MV
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

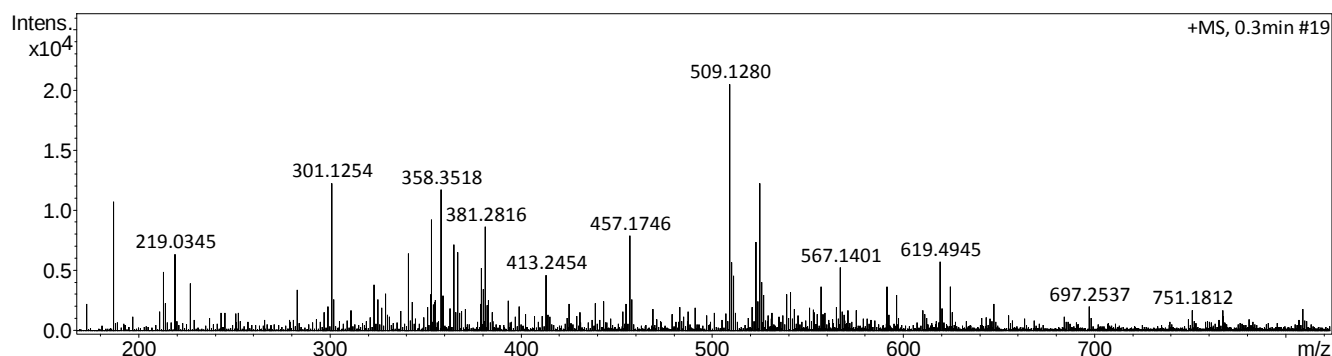

#	m/z	I	I %
1	187.0322	10679	52.3
2	213.0642	4869	23.8
3	219.0345	6330	31.0
4	226.9427	3912	19.1
5	283.0832	3375	16.5
6	301.1254	12234	59.9
7	323.0655	3792	18.6
8	329.0560	3045	14.9
9	341.0743	6382	31.2
10	353.2479	9176	44.9
11	358.3518	11694	57.2
12	365.1110	7139	34.9
13	367.1150	6491	31.8
14	379.2613	5166	25.3
15	380.3226	3415	16.7
16	381.2816	8595	42.1
17	413.2454	4609	22.6
18	457.1746	7876	38.6
19	509.1280	20429	100.0
20	510.1327	5638	27.6
21	511.1376	4564	22.3
22	523.1077	7370	36.1
23	525.1218	12192	59.7
24	526.1238	4028	19.7
25	541.1111	3142	15.4
26	557.0976	3667	17.9
27	567.1401	5241	25.7
28	591.4679	3633	17.8
29	619.4945	5707	27.9
30	624.5951	3664	17.9