

Mass Spectrum List Report

Analysis Info

Analysis Name D:\Data\ggc\HG-3L_P1-C-8_01_9830.d
 Method lc_ms directos tunelow300924.m
 Sample Name HG-3L
 Comment Sv: MeOH + HCOOH
 Szajnman


Acquisition Date 12/23/2024 1:21:50 PM

Operator EB - MV

Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

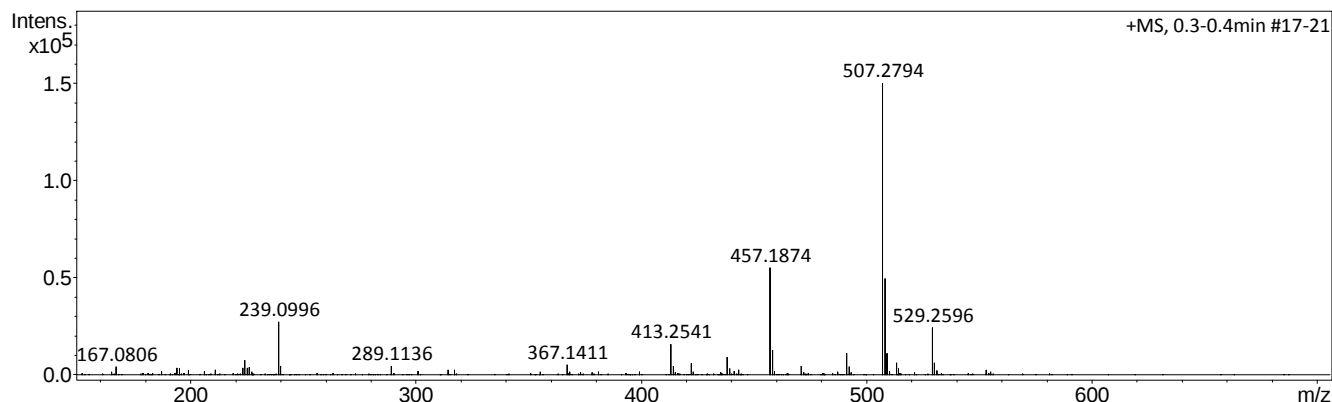

#	m/z	I	I %
1	167.0806	4391	2.9
2	194.0898	3581	2.4
3	195.0798	3372	2.2
4	211.0732	2702	1.8
5	223.1054	3602	2.4
6	224.1141	7510	5.0
7	225.0909	3656	2.4
8	226.0901	4142	2.8
9	239.0996	27472	18.3
10	240.1026	4652	3.1
11	289.1136	4571	3.0
12	367.1411	5408	3.6
13	413.2541	15861	10.6
14	414.2516	4715	3.1
15	422.2148	6037	4.0
16	438.2067	9416	6.3
17	439.2130	3259	2.2
18	457.1874	55196	36.8
19	458.1905	12752	8.5
20	471.1679	4581	3.1
21	491.2824	11236	7.5
22	492.2900	4341	2.9
23	507.2794	149990	100.0
24	508.2842	49776	33.2
25	509.2807	11387	7.6
26	513.2663	6433	4.3
27	514.2722	3461	2.3
28	529.2596	24399	16.3
29	530.2582	6271	4.2
30	553.2060	2848	1.9