

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\HG-3L1_P1-C-5_01_9990.d
 Method lc_ms directos tunelow300924.m
 Sample Name HG-3L1
 Comment Sv: MeOH
 Szajnman

Acquisition Date 1/15/2025 3:45:52 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1200 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

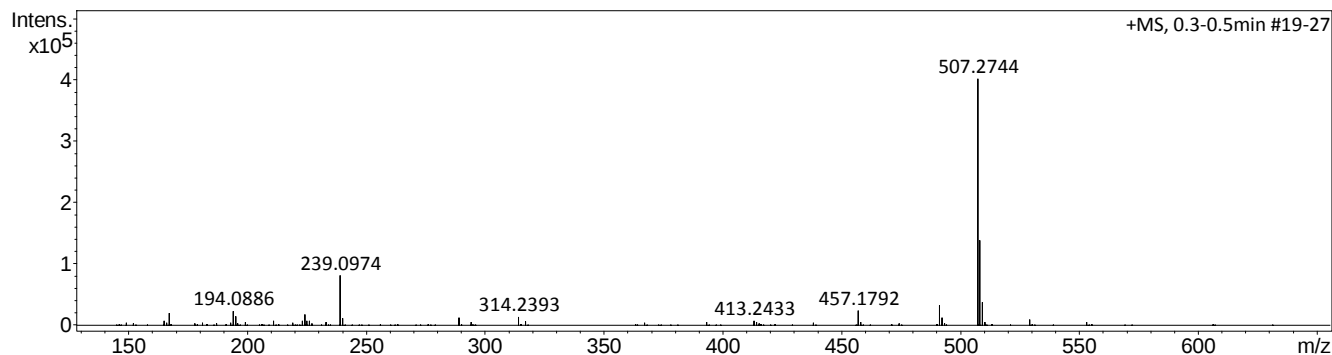

#	m/z	I	I %
1	165.0621	7180	1.8
2	167.0776	19995	5.0
3	194.0886	22670	5.7
4	195.0768	15069	3.8
5	199.0670	5640	1.4
6	211.0667	7693	1.9
7	223.1016	7467	1.9
8	224.1115	18368	4.6
9	225.0921	7463	1.9
10	226.0906	7285	1.8
11	233.0952	5123	1.3
12	239.0974	80999	20.2
13	240.1035	11769	2.9
14	289.1124	12672	3.2
15	294.1742	5614	1.4
16	314.2393	13761	3.4
17	317.1408	7005	1.7
18	393.2104	5091	1.3
19	413.2433	8064	2.0
20	414.2431	5138	1.3
21	457.1792	24164	6.0
22	458.1824	5390	1.3
23	491.2762	32560	8.1
24	492.2898	12737	3.2
25	507.2744	401037	100.0
26	508.2784	138767	34.6
27	509.2753	37802	9.4
28	510.2817	5962	1.5
29	529.2556	9308	2.3
30	553.1968	5290	1.3