

Mass Spectrum List Report

Analysis Info

Analysis Name D:\Data\ggc\HG-3L2_P1-D-6_01_10046.d
 Method lc_ms directos tunelow300924.m
 Sample Name HG-3L2
 Comment Sv: MeOH
 Szajnman


Acquisition Date 2/14/2025 2:30:11 PM

Operator EB - MV

Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1200 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

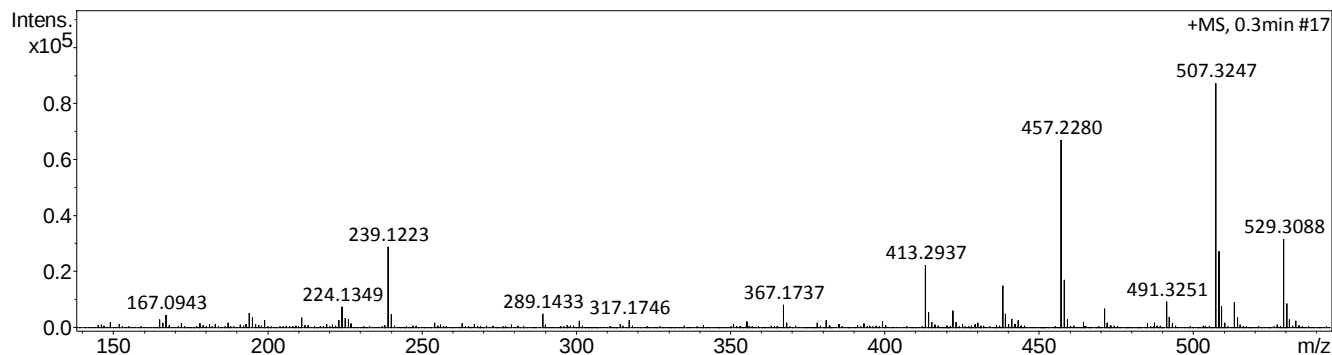

#	m/z	I	I %
1	167.0943	4506	5.2
2	194.1087	5029	5.8
3	195.0968	3494	4.0
4	211.0913	3500	4.0
5	224.1349	7304	8.4
6	225.1137	3380	3.9
7	226.1139	2916	3.4
8	239.1223	28883	33.2
9	240.1272	4698	5.4
10	289.1433	5020	5.8
11	367.1737	8056	9.3
12	413.2937	22171	25.5
13	414.2929	5368	6.2
14	422.2521	6053	7.0
15	438.2500	14836	17.1
16	439.2530	4839	5.6
17	441.3218	3187	3.7
18	457.2280	66876	76.9
19	458.2339	16885	19.4
20	471.2103	6779	7.8
21	491.3251	9244	10.6
22	492.3358	3746	4.3
23	507.3247	86976	100.0
24	508.3317	27139	31.2
25	509.3253	7591	8.7
26	513.3104	9099	10.5
27	514.3177	3461	4.0
28	529.3088	31425	36.1
29	530.3106	8656	10.0
30	531.3134	2875	3.3