

Mass Spectrum List Report

Analysis Info

Analysis Name D:\Data\ggc\HG-3X2_P1-D-4_01_10047.d
 Method lc ms directos_241016neg.m
 Sample Name HG-3X2
 Comment Sv: MeOH
 Szajnman


Acquisition Date 2/14/2025 3:05:03 PM

Operator EB - MV

Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Negative	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	3500 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

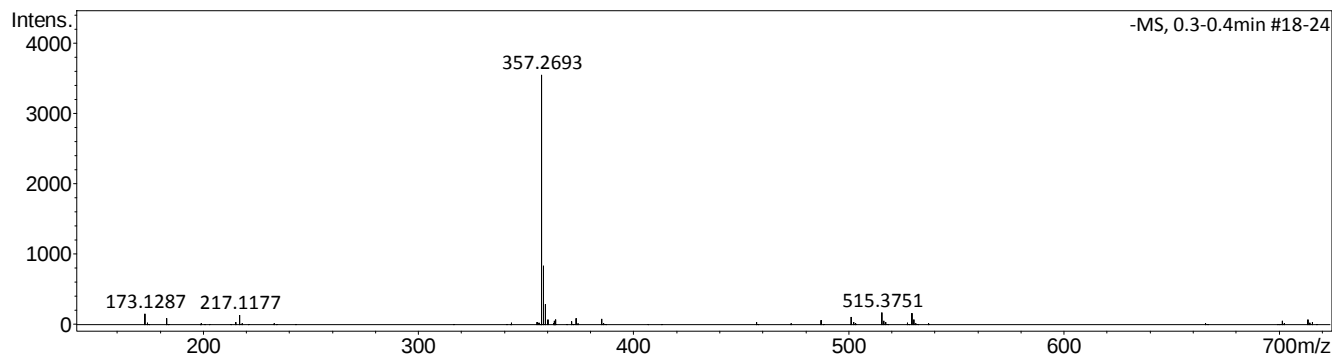

#	m/z	I	I %
1	173.1287	149	4.2
2	183.1314	84	2.4
3	215.1031	31	0.9
4	217.1177	129	3.6
5	355.2624	36	1.0
6	357.2693	3540	100.0
7	358.2706	830	23.5
8	359.2687	288	8.1
9	360.2684	66	1.9
10	363.2300	50	1.4
11	363.6305	39	1.1
12	363.7431	65	1.8
13	371.2754	40	1.1
14	373.2627	87	2.5
15	385.3014	80	2.3
16	457.1865	36	1.0
17	487.3450	59	1.7
18	501.3633	109	3.1
19	502.3689	36	1.0
20	515.3751	171	4.8
21	516.3687	50	1.4
22	517.3801	36	1.0
23	527.3774	25	0.7
24	529.3891	155	4.4
25	530.3915	73	2.1
26	701.4976	53	1.5
27	713.5253	67	1.9
28	714.5334	28	0.8
29	715.5199	33	0.9
30	938.8126	60	1.7