

Mass Spectrum List Report

Analysis Info

Analysis Name D:\Data\ggc\HG-3X2_P1-D-4_01_10044.d
 Method lc_ms directos tunelow300924.m
 Sample Name HG-3X2
 Comment Sv: MeOH
 Szajnman


Acquisition Date 2/14/2025 2:19:55 PM

Operator EB - MV

Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1200 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

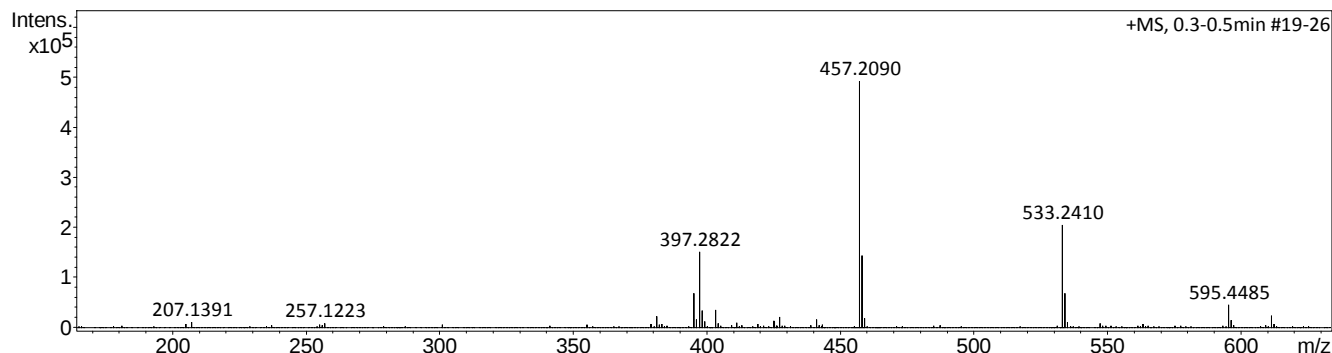

#	m/z	I	I %
1	205.1230	7096	1.4
2	207.1391	11380	2.3
3	257.1223	8371	1.7
4	379.2678	7242	1.5
5	381.2742	22070	4.5
6	383.2662	7370	1.5
7	395.2674	68554	14.0
8	396.2695	16047	3.3
9	397.2822	151491	30.9
10	398.2854	33692	6.9
11	399.2890	11675	2.4
12	403.2716	35081	7.1
13	404.2727	8608	1.8
14	411.2989	9201	1.9
15	419.2656	6985	1.4
16	425.1455	12979	2.6
17	425.3120	12650	2.6
18	427.2930	20689	4.2
19	441.3074	16607	3.4
20	457.2090	490746	100.0
21	458.2127	142662	29.1
22	459.2137	18719	3.8
23	533.2410	204582	41.7
24	534.2476	68191	13.9
25	535.2431	11407	2.3
26	547.3850	8291	1.7
27	595.4485	45853	9.3
28	596.4497	15131	3.1
29	611.4419	23541	4.8
30	612.4433	7598	1.5