

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\HG-3a_P1-B-9_01_9822.d
 Method lc_ms directos tunelow300924.m
 Sample Name HG-3a
 Comment Sv: MeOH + HCOOH
 Szajnman

Acquisition Date 12/23/2024 12:40:46 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

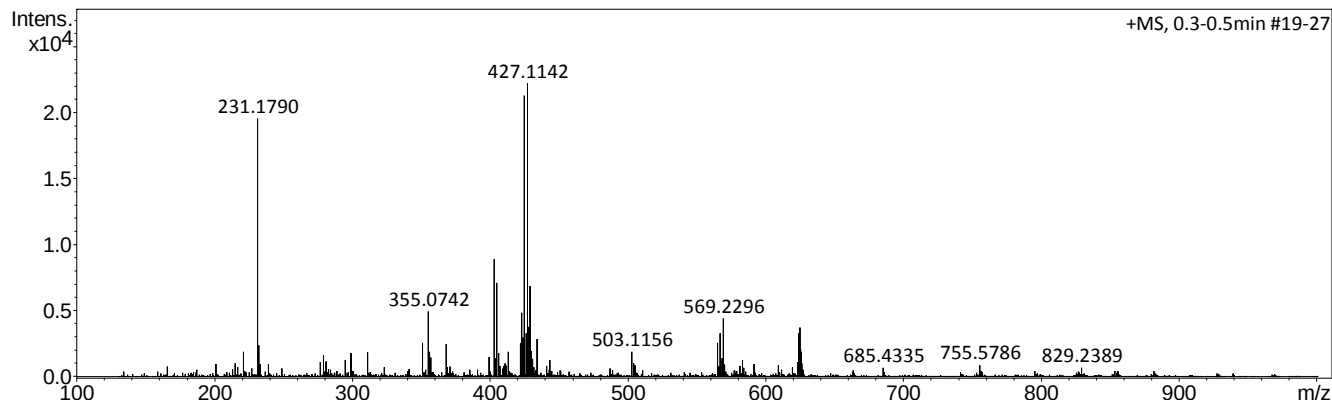

#	m/z	I	I %
1	221.0878	1882	8.5
2	231.1790	19487	87.9
3	232.1817	2372	10.7
4	351.1110	2570	11.6
5	355.0742	4942	22.3
6	355.2827	2045	9.2
7	368.4244	2473	11.2
8	403.1358	8864	40.0
9	405.1302	7096	32.0
10	413.2719	1909	8.6
11	422.1087	2513	11.3
12	423.1066	4819	21.7
13	423.6105	1999	9.0
14	424.1046	2947	13.3
15	425.1178	21222	95.8
16	426.1216	3274	14.8
17	427.1142	22160	100.0
18	428.1148	3791	17.1
19	429.0982	6864	31.0
20	430.0922	1935	8.7
21	434.1123	2834	12.8
22	503.1156	1906	8.6
23	565.1999	2573	11.6
24	567.2364	3306	14.9
25	569.2296	4407	19.9
26	624.1730	3292	14.9
27	624.6753	2036	9.2
28	625.1734	3731	16.8
29	625.6744	2103	9.5
30	626.1739	1887	8.5