

Mass Spectrum List Report

Analysis Info

Analysis Name D:\Data\ggc\HG-3a1_P1-C-1_01_9986.d
 Method lc_ms directos tunelow300924.m
 Sample Name HG-3a1
 Comment Sv: MeOH
 Szajnman


Acquisition Date 1/15/2025 3:25:20 PM

Operator EB - MV

Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1200 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

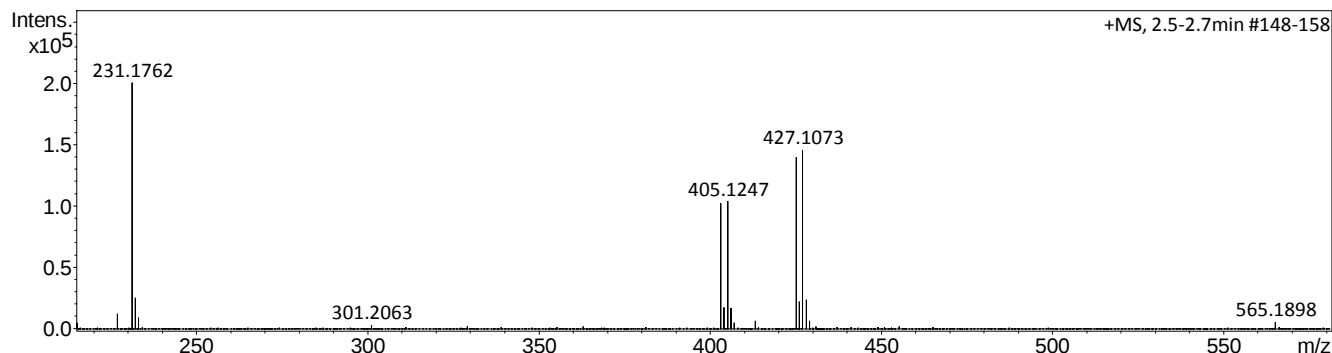

#	m/z	I	I %
1	134.0718	3711	1.9
2	149.0235	1974	1.0
3	158.9625	2193	1.1
4	166.0447	3776	1.9
5	184.0704	1765	0.9
6	184.9582	2854	1.4
7	186.9565	2594	1.3
8	212.9882	4091	2.0
9	214.9869	3719	1.9
10	215.1809	5130	2.6
11	226.9489	12055	6.0
12	231.1762	200538	100.0
13	232.1766	25046	12.5
14	233.1739	9205	4.6
15	301.2063	2680	1.3
16	362.9242	1802	0.9
17	403.1281	101915	50.8
18	404.1317	17311	8.6
19	405.1247	103445	51.6
20	406.1265	16783	8.4
21	407.1245	4918	2.5
22	413.2637	6379	3.2
23	425.1082	139602	69.6
24	426.1130	22136	11.0
25	427.1073	145216	72.4
26	428.1110	23451	11.7
27	429.1050	6326	3.2
28	430.9080	1989	1.0
29	565.1898	5441	2.7
30	829.2199	2784	1.4