

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\HG-3e_P1-C-2_01_9987.d
 Method lc_ms directos tunelow300924.m
 Sample Name HG-3e
 Comment Sv: MeOH
 Szajnman

Acquisition Date 1/15/2025 3:30:27 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1200 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

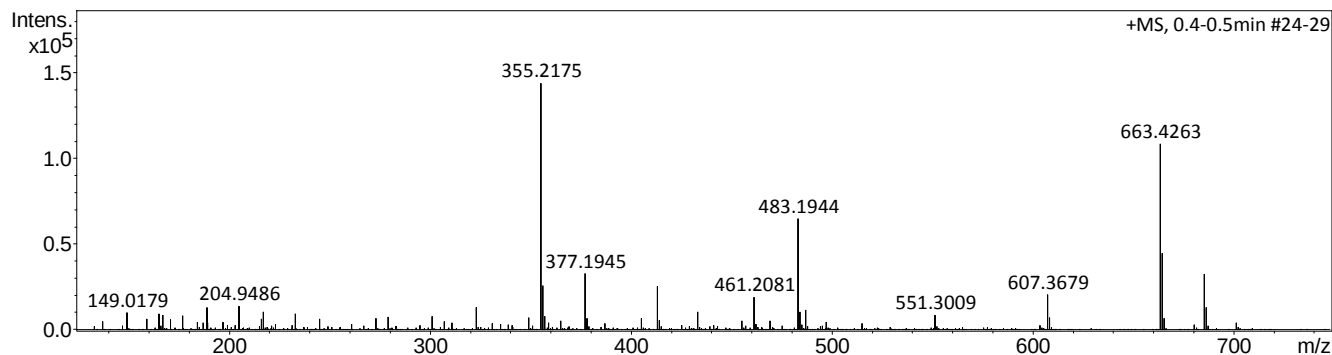

#	m/z	I	I %
1	149.0179	10265	7.1
2	165.0727	9468	6.6
3	167.0467	8468	5.9
4	176.9645	8413	5.9
5	188.9648	13122	9.1
6	204.9486	14037	9.8
7	216.9969	10646	7.4
8	232.9760	9534	6.6
9	278.9527	7452	5.2
10	301.0924	7791	5.4
11	323.0697	13101	9.1
12	349.0872	7292	5.1
13	355.2175	143748	100.0
14	356.2199	25873	18.0
15	357.2146	7719	5.4
16	377.1945	32630	22.7
17	413.2540	25278	17.6
18	433.1797	10451	7.3
19	461.2081	18884	13.1
20	483.1944	64922	45.2
21	484.1991	10433	7.3
22	487.1247	11748	8.2
23	551.3009	8464	5.9
24	607.3679	20670	14.4
25	608.3705	7316	5.1
26	663.4263	108247	75.3
27	664.4328	44736	31.1
28	665.4356	6847	4.8
29	685.4083	32414	22.5
30	686.4123	13076	9.1