

Mass Spectrum List Report

Analysis Info

Analysis Name D:\Data\ggc\HG-3m_P1-C-9_01_9886.d
 Method lc-ms directos tunelow261224 apci.m
 Sample Name HG-3m
 Comment Sv: MeOH + HCOOH
 Szajnman


Acquisition Date 12/26/2024 4:07:02 PM

Operator EB - MV

Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	APCI	Ion Polarity	Positive	Set Nebulizer	1.6 Bar
Focus	Not active	Set Capillary	4500 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	8.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

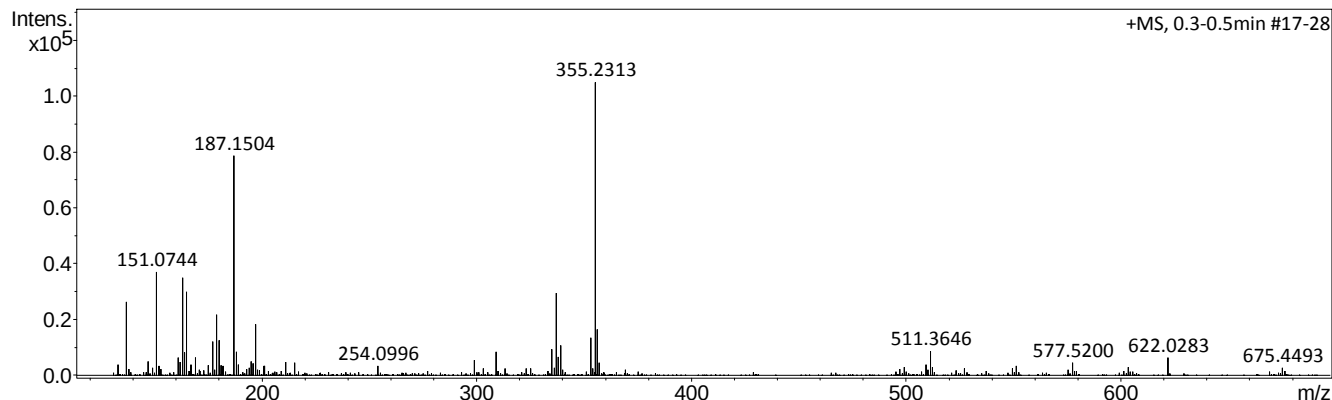

#	m/z	I	I %
1	137.0588	26240	25.1
2	147.0794	5022	4.8
3	151.0744	36988	35.3
4	161.0625	6452	6.2
5	162.0671	4751	4.5
6	163.0739	34885	33.3
7	164.0819	8313	7.9
8	165.0454	29882	28.6
9	169.0324	6355	6.1
10	177.0885	12170	11.6
11	179.0664	21773	20.8
12	180.0770	12673	12.1
13	187.1504	78588	75.1
14	188.1529	8375	8.0
15	195.0502	5064	4.8
16	197.0619	18238	17.4
17	211.0765	4932	4.7
18	215.1812	4540	4.3
19	299.1285	5603	5.4
20	309.1911	8371	8.0
21	335.2038	9389	9.0
22	337.2179	29411	28.1
23	338.2240	6737	6.4
24	339.2342	10782	10.3
25	353.2289	13582	13.0
26	355.2313	104658	100.0
27	356.2349	16435	15.7
28	357.2347	4715	4.5
29	511.3646	8738	8.3
30	622.0283	6362	6.1