

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\HG-3n_P1-D-1_01_9832.d
 Method lc_ms directos tunelow300924.m
 Sample Name HG-3n
 Comment Sv: MeOH + HCOOH
 Szajnman

Acquisition Date 12/23/2024 1:32:05 PM

Operator EB - MV
 Instrument micrOTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

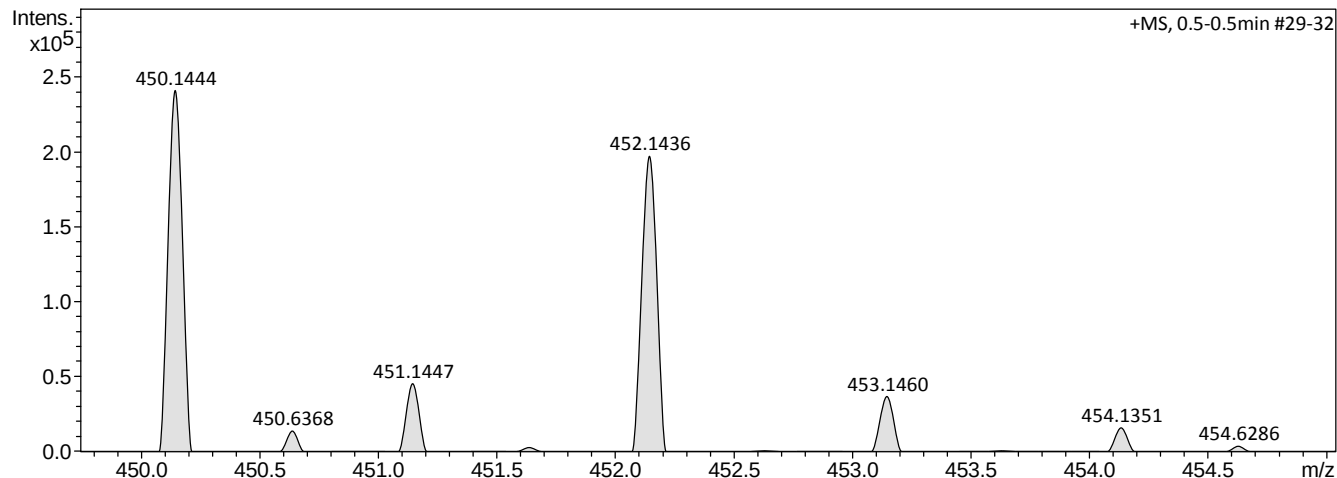

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
450.1444	1	C21H34BrNNaOS	450.1437	-1.6	134.4	2	8.96	4.5	even	ok