

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\HG-3q_P1-D-3_01_9885.d
 Method lc-ms directos tunelow261224 apci.m
 Sample Name HG-3q
 Comment Sv: MeOH + HCOOH
 Szajnman

Acquisition Date 12/26/2024 4:01:54 PM

Operator EB - MV
 Instrument micrOTOF-Q

Acquisition Parameter

Source Type	APCI	Ion Polarity	Positive	Set Nebulizer	1.6 Bar
Focus	Not active	Set Capillary	4500 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	8.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

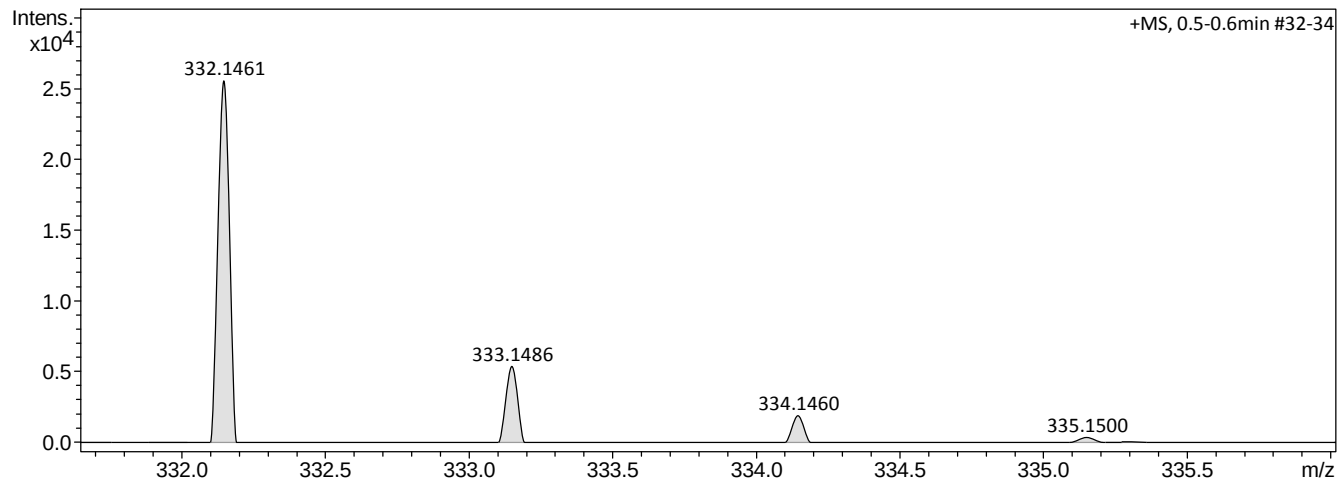

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
332.1461	1	C22H22NS	332.1467	1.9	21.3	1	100.00	12.5	even	ok