

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\HG-3u_P1-C-7_01_9992.d
 Method lc_ms directos tunelow300924.m
 Sample Name HG-3u
 Comment Sv: MeOH
 Szajnman

Acquisition Date 1/15/2025 3:56:06 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1200 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

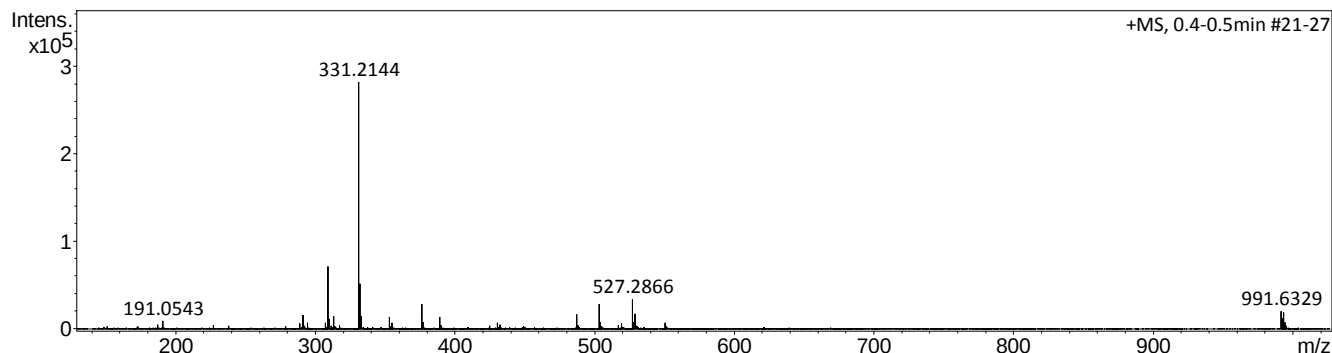

#	m/z	I	I %
1	187.1548	5054	1.8
2	191.0543	9437	3.4
3	289.2057	5864	2.1
4	291.2183	16008	5.7
5	294.3203	7017	2.5
6	307.3176	6756	2.4
7	309.2310	70832	25.2
8	310.2333	11106	4.0
9	313.2993	13971	5.0
10	331.2144	281111	100.0
11	332.2187	51195	18.2
12	333.2119	14150	5.0
13	353.1408	13205	4.7
14	355.1413	6800	2.4
15	376.3987	27974	10.0
16	377.4038	7671	2.7
17	389.3954	13523	4.8
18	430.4488	7165	2.5
19	487.3488	16467	5.9
20	503.3426	28322	10.1
21	504.3481	7393	2.6
22	519.3372	6007	2.1
23	527.2866	33568	11.9
24	528.2933	7914	2.8
25	529.2839	17292	6.2
26	550.5425	7181	2.6
27	991.6329	19952	7.1
28	992.6341	11860	4.2
29	993.6380	18686	6.6
30	994.6397	7315	2.6