

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\HG-3x_P1-D-4_01_9896.d
Method lc ms directos_241016neg.m
Sample Name HG-3x
Comment Sv: MeOH + HCOOH
Szajnman

Acquisition Date 12/30/2024 1:18:24 PM

Operator EB - MV
Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Negative	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	3500 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

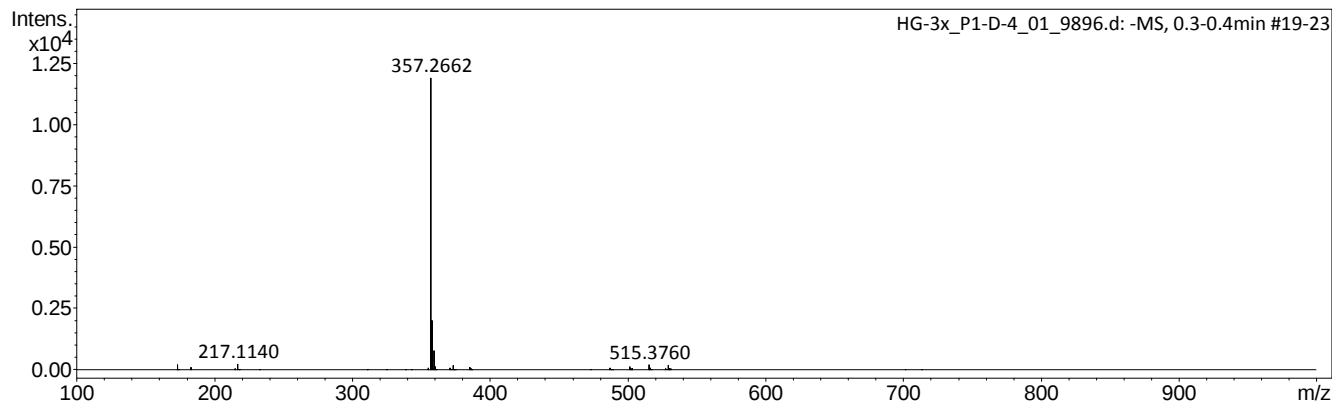

#	m/z	I	I %
1	173.1292	210	1.8
2	183.1316	96	0.8
3	215.1008	56	0.5
4	217.1140	230	1.9
5	218.1173	32	0.3
6	233.1106	37	0.3
7	355.2502	84	0.7
8	357.2662	11882	100.0
9	358.2689	2015	17.0
10	359.2651	780	6.6
11	360.2662	129	1.1
12	361.2697	28	0.2
13	371.2709	92	0.8
14	373.2571	196	1.6
15	374.2640	36	0.3
16	385.2973	116	1.0
17	386.2932	43	0.4
18	387.2927	28	0.2
19	487.3390	74	0.6
20	501.3596	119	1.0
21	502.3517	47	0.4
22	503.3573	43	0.4
23	515.3760	209	1.8
24	516.3700	79	0.7
25	527.3716	48	0.4
26	529.3870	191	1.6
27	530.3891	66	0.6
28	531.3890	53	0.4
29	701.5129	36	0.3
30	713.5348	31	0.3