

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\HG-3y_P1-C-6_01_9991.d
 Method lc_ms directos tunelow300924.m
 Sample Name HG-3y
 Comment Sv: MeOH
 Szajnman

Acquisition Date 1/15/2025 3:50:58 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1200 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

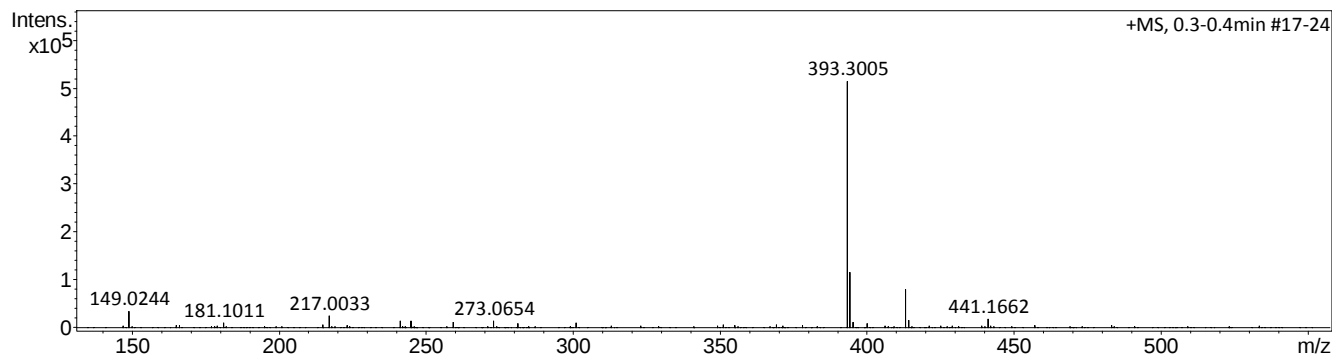

#	m/z	I	I %
1	149.0244	33962	6.6
2	165.0705	4492	0.9
3	166.0783	5009	1.0
4	181.1011	10921	2.1
5	214.9880	5769	1.1
6	217.0033	24894	4.8
7	223.0620	5590	1.1
8	241.1830	14284	2.8
9	245.0358	13818	2.7
10	259.1908	12192	2.4
11	273.0654	13950	2.7
12	281.1725	9195	1.8
13	301.0997	10843	2.1
14	323.0806	4293	0.8
15	351.1079	6136	1.2
16	355.0706	4723	0.9
17	369.1280	6268	1.2
18	378.1019	4639	0.9
19	393.3005	513879	100.0
20	394.3012	115743	22.5
21	395.3066	12116	2.4
22	400.0862	9685	1.9
23	413.2697	79864	15.5
24	414.2688	16079	3.1
25	425.1332	4339	0.8
26	441.1662	18977	3.7
27	442.1718	4197	0.8
28	457.1931	4975	1.0
29	483.2083	5206	1.0
30	533.4579	3857	0.8