

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\HG-C5_P1-C-8_01_10021.d
 Method lc_ms directos tunelow300924.m
 Sample Name HG-C5
 Comment Sv: MeOH
 Szajnman

Acquisition Date 2/11/2025 1:39:31 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1200 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

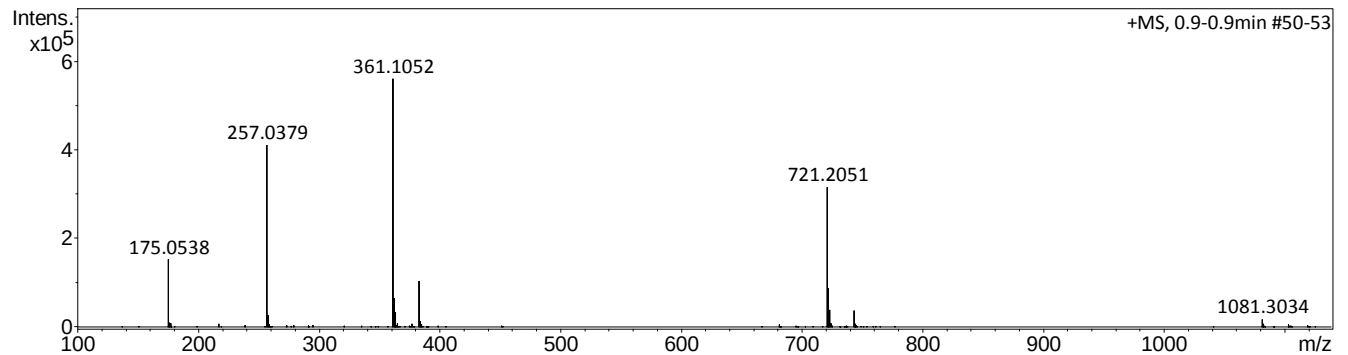

#	m/z	I	I %
1	175.0538	152787	27.3
2	176.0572	9255	1.7
3	177.0681	7973	1.4
4	217.0053	6949	1.2
5	239.0248	4632	0.8
6	257.0379	409768	73.3
7	258.0410	26566	4.8
8	259.0428	4771	0.9
9	273.0159	4718	0.8
10	291.0242	3796	0.7
11	294.9971	3974	0.7
12	361.1052	559059	100.0
13	362.1074	64170	11.5
14	363.1027	32173	5.8
15	365.0748	7994	1.4
16	377.1026	6219	1.1
17	383.0859	103985	18.6
18	384.0905	12062	2.2
19	385.0837	5182	0.9
20	681.1781	5373	1.0
21	721.2051	314887	56.3
22	722.2065	88202	15.8
23	723.2050	37957	6.8
24	724.2061	8345	1.5
25	743.1881	36572	6.5
26	744.1837	7557	1.4
27	745.1896	3721	0.7
28	1081.3034	17196	3.1
29	1082.3054	6947	1.2
30	1103.2851	5685	1.0