

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\SJ222P_P1-D-1_01_9158.d
 Method lc_qtof_directospos.m
 Sample Name SJ222P
 Comment Sv: MeOH + HCOOH
 Szajnman

Acquisition Date 5/6/2024 3:53:12 PM

Operator ELB
 Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

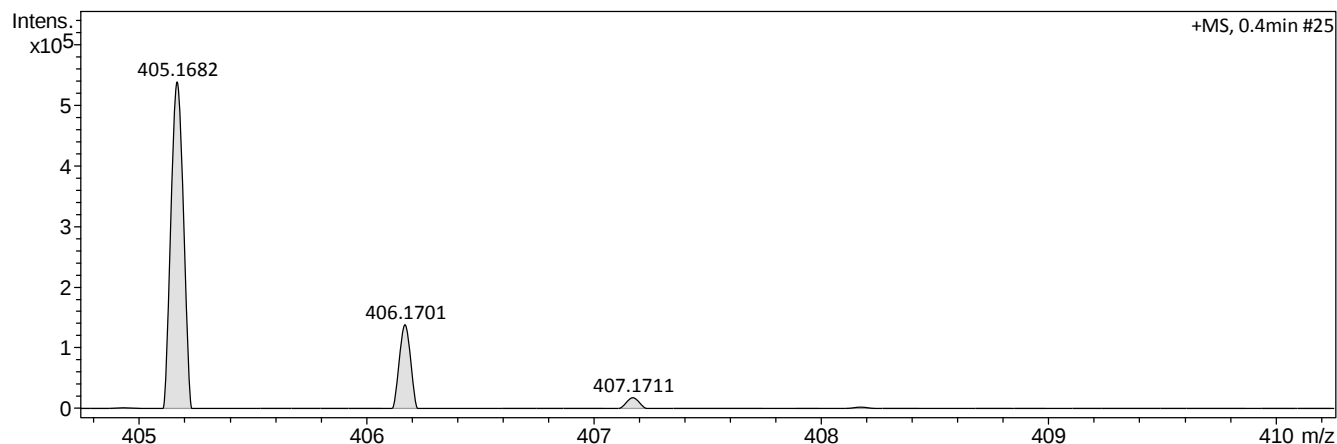

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
405.1682	1	C23H26NaO5	405.1672	-2.3	4.2	1	69.63	10.5	even	ok