

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\VL-79p_P1-B-6_01_9661.d
 Method lc_ms directos tunelow300924.m
 Sample Name VL-79p
 Comment Sv: MeOH + HCOOH
 Sergio Szajman

Acquisition Date 11/8/2024 1:10:00 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

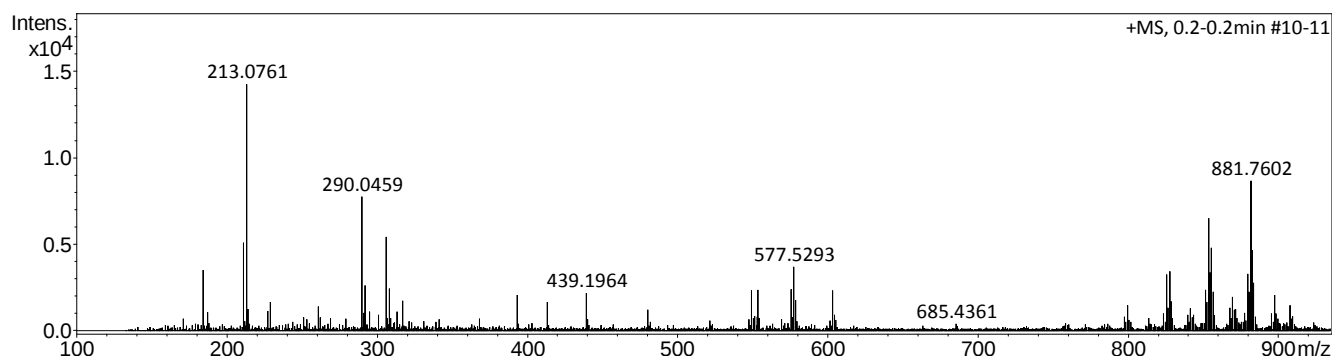

#	m/z	I	I %
1	184.0768	3514	24.7
2	211.0956	5090	35.8
3	213.0761	14225	100.0
4	290.0459	7738	54.4
5	292.0439	2613	18.4
6	306.0189	5402	38.0
7	308.0170	2425	17.1
8	317.1703	1722	12.1
9	393.3031	2085	14.7
10	439.1964	2177	15.3
11	549.4962	2318	16.3
12	553.4675	2352	16.5
13	575.5066	2408	16.9
14	577.5293	3699	26.0
15	578.5313	1768	12.4
16	603.5444	2313	16.3
17	825.7026	3230	22.7
18	827.7251	3422	24.1
19	851.7200	2363	16.6
20	853.7325	6467	45.5
21	854.7357	3362	23.6
22	855.7456	4791	33.7
23	856.7553	2266	15.9
24	869.7202	1967	13.8
25	879.7506	3291	23.1
26	880.7618	2258	15.9
27	881.7602	8639	60.7
28	882.7696	4656	32.7
29	883.7796	2762	19.4
30	897.7340	2050	14.4