

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\VL-97_P1-D-3_01_9232.d
 Method lc_qtof_directospos.m
 Sample Name VL-97
 Comment Sv: MeOH + HCOOH
 Szajnman

Acquisition Date 6/6/2024 3:02:56 PM

Operator MV
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

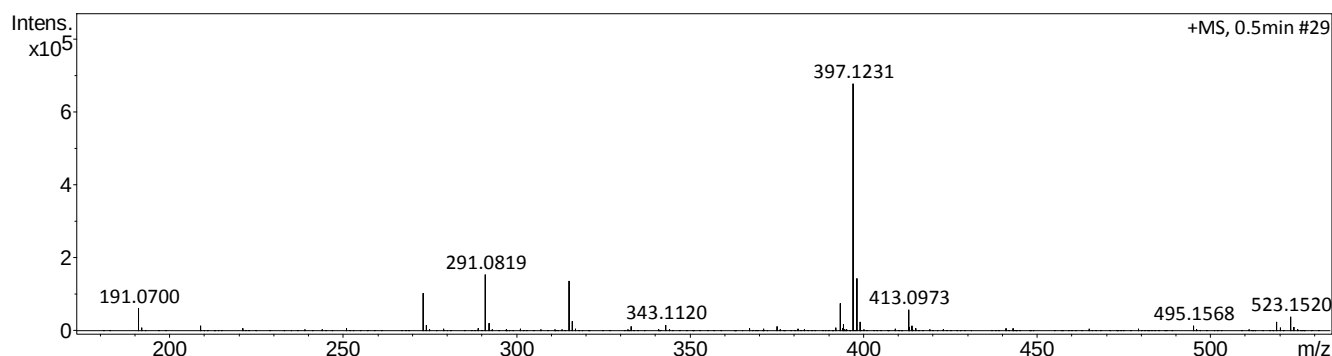

#	m/z	I	I %
1	191.0700	61673	9.1
2	192.0733	7895	1.2
3	209.0807	13996	2.1
4	273.0725	103523	15.3
5	274.0753	14606	2.2
6	291.0819	153065	22.6
7	292.0859	20976	3.1
8	315.1211	136177	20.1
9	316.1247	26649	3.9
10	333.0933	11455	1.7
11	343.1120	14729	2.2
12	375.1416	11916	1.8
13	392.1670	8252	1.2
14	393.2946	74694	11.0
15	394.2952	17675	2.6
16	397.1231	676285	100.0
17	398.1253	143688	21.2
18	399.1272	24308	3.6
19	413.0973	57571	8.5
20	413.2598	9580	1.4
21	414.0993	13105	1.9
22	495.1568	13660	2.0
23	519.1583	24227	3.6
24	520.1648	7577	1.1
25	523.1520	37709	5.6
26	524.1589	10432	1.5
27	541.1604	7974	1.2
28	647.2039	9371	1.4
29	771.2568	49257	7.3
30	772.2623	22940	3.4