

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\shs-1_P1-E-7_01_9895.d
 Method lc_ms directos tunelow300924.m
 Sample Name shs-1
 Comment Sv: MeOH + HCOOH
 Szajnman

Acquisition Date 12/30/2024 12:41:59 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1200 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

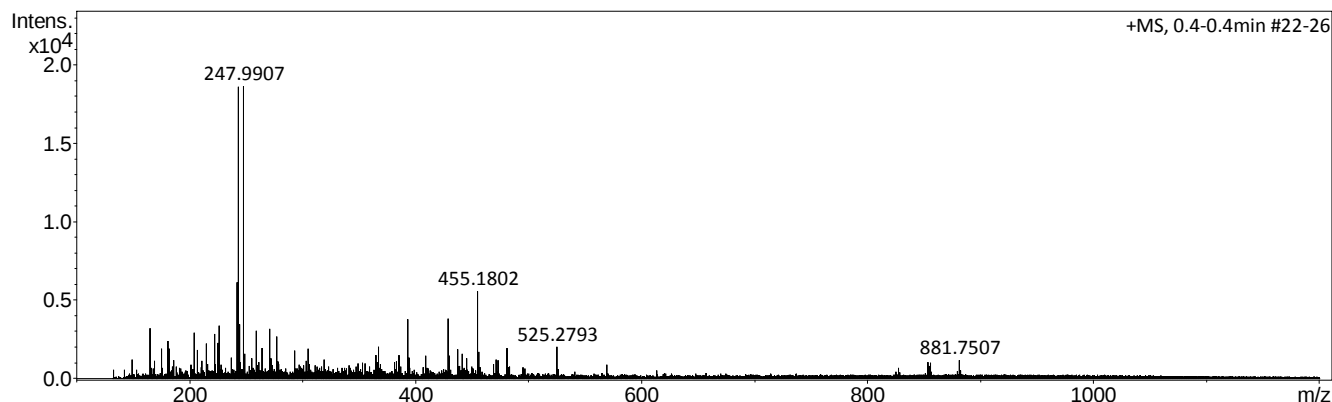

#	m/z	I	I %
1	165.0703	3217	17.3
2	174.9991	1912	10.3
3	181.0528	2415	13.0
4	182.0272	1898	10.2
5	204.0069	2910	15.7
6	207.0267	1832	9.9
7	215.0991	2220	11.9
8	222.0137	2837	15.3
9	224.9805	2260	12.2
10	226.0048	3395	18.3
11	242.2832	6149	33.1
12	243.1171	18580	100.0
13	244.1172	3442	18.5
14	247.9907	18589	100.0
15	248.9984	1604	8.6
16	259.0707	3034	16.3
17	263.9689	1957	10.5
18	271.0702	3159	17.0
19	277.0776	2702	14.5
20	293.0557	1786	9.6
21	305.0899	1920	10.3
22	367.1415	2044	11.0
23	393.1797	3787	20.4
24	429.1627	3813	20.5
25	437.2290	1888	10.2
26	441.1577	1588	8.5
27	455.1802	5569	30.0
28	456.1826	1705	9.2
29	481.2434	1969	10.6
30	525.2793	2036	11.0