

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\25-020310_P1-C-1_01_10057.d
 Method lc_ms directos tunelow300924.m
 Sample Name 25-020310
 Comment NFC-FAZT1(may)
 Sv: MeOH + HCOOH
 Uhrig

Acquisition Date 2/24/2025 3:18:41 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1200 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

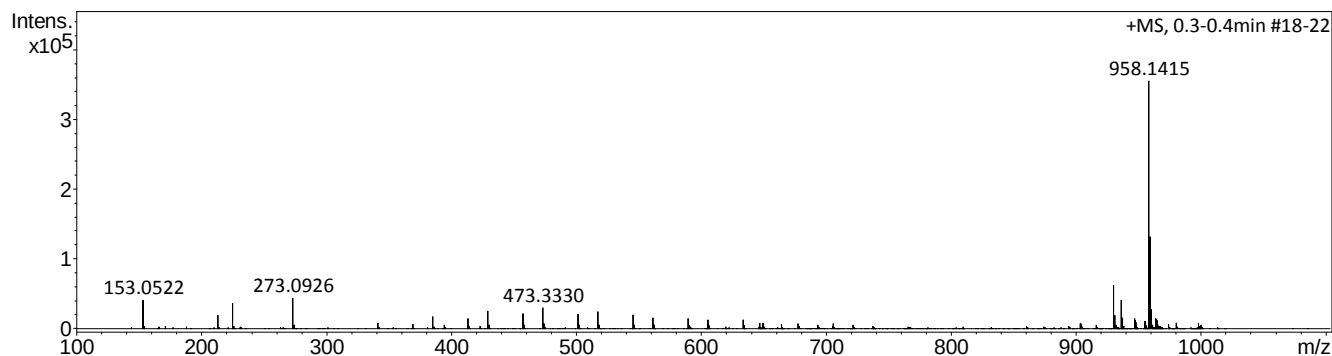

#	m/z	I	I %
1	153.0522	40998	11.6
2	213.0729	19780	5.6
3	225.0844	36892	10.4
4	273.0926	44207	12.5
5	385.2864	17068	4.8
6	413.3046	15006	4.2
7	429.3094	25833	7.3
8	457.3421	21680	6.1
9	473.3330	30050	8.5
10	501.3635	21569	6.1
11	517.3596	24785	7.0
12	545.3911	20201	5.7
13	561.3859	15808	4.5
14	589.4169	14853	4.2
15	605.4103	13030	3.7
16	633.4450	12835	3.6
17	930.1358	61983	17.5
18	931.1433	19106	5.4
19	936.1589	41058	11.6
20	937.1601	15486	4.4
21	947.1460	14340	4.0
22	947.6538	12295	3.5
23	955.1384	11277	3.2
24	955.6408	9891	2.8
25	958.1415	354572	100.0
26	959.1451	131363	37.0
27	960.1458	28799	8.1
28	964.1246	15084	4.3
29	964.6276	12666	3.6
30	965.1204	11948	3.4