

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\25-020311_P1-C-2_01_10058.d
 Method lc_ms directos tunelow300924.m
 Sample Name 25-020311
 Comment NFC-FAZT1(min)
 Sv: MeOH + HCOOH
 Uhrig

Acquisition Date 2/24/2025 3:23:50 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1200 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

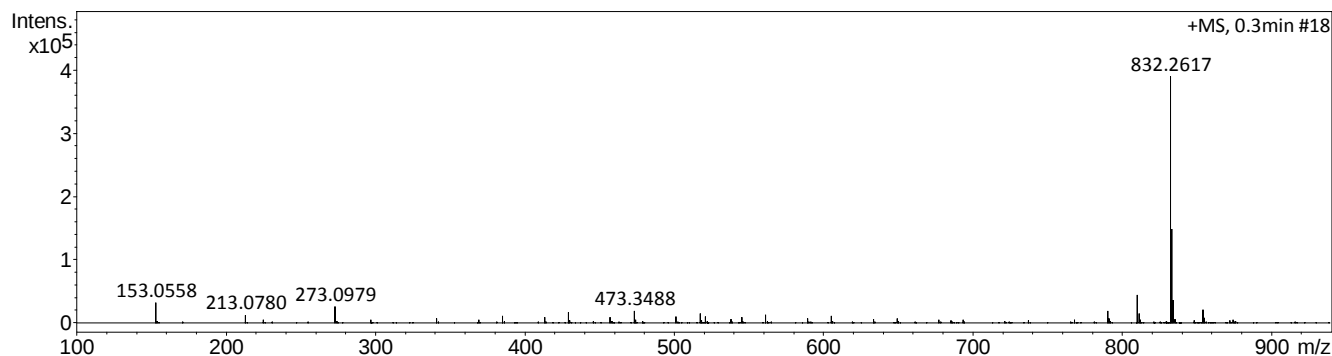

#	m/z	I	I %
1	153.0558	32157	8.3
2	213.0780	12283	3.2
3	273.0979	26204	6.7
4	341.2692	7380	1.9
5	385.2963	11340	2.9
6	413.3149	9125	2.3
7	429.3228	17607	4.5
8	457.3528	8854	2.3
9	473.3488	19162	4.9
10	501.3804	10430	2.7
11	517.3772	15557	4.0
12	521.1650	10525	2.7
13	538.1944	6110	1.6
14	545.4127	8786	2.3
15	561.3973	13046	3.3
16	589.4335	6851	1.8
17	605.4328	11634	3.0
18	633.4714	6602	1.7
19	649.4517	7327	1.9
20	790.2512	19178	4.9
21	791.2629	7336	1.9
22	810.2749	43946	11.3
23	811.2792	14945	3.8
24	832.2617	389592	100.0
25	833.2659	148698	38.2
26	834.2670	36587	9.4
27	835.2610	6360	1.6
28	854.2454	21361	5.5
29	855.2522	7960	2.0
30	958.1426	6022	1.5