

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\25-020311_P1-C-2_01_10058.d
 Method lc_ms directos tunelow300924.m
 Sample Name 25-020311
 Comment NFC-FAZT1(min)
 Sv: MeOH + HCOOH
 Uhrig

Acquisition Date 2/24/2025 3:23:50 PM

Operator EB - MV
 Instrument micrOTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1200 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

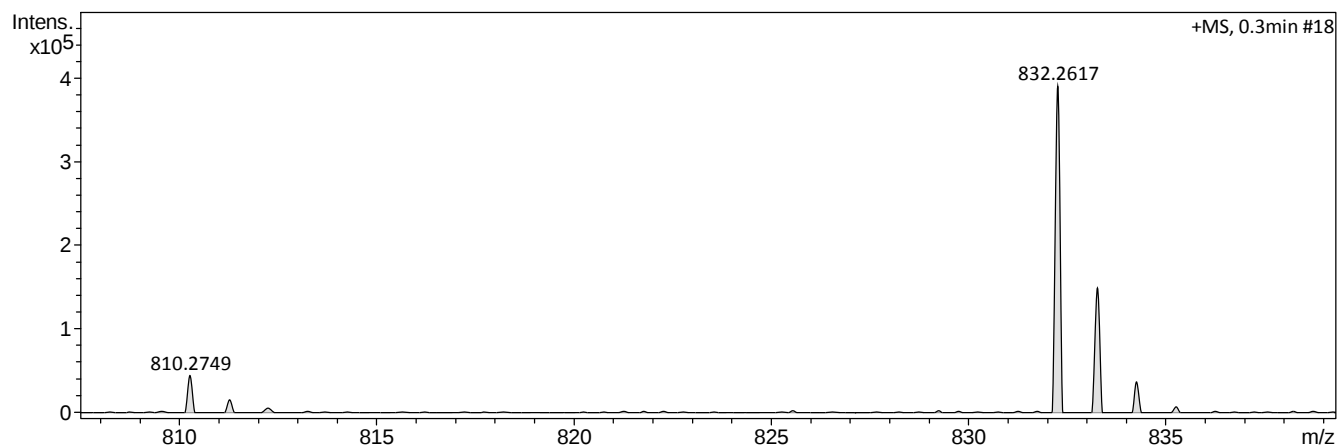

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
810.2749	1	C33H44N7O17	810.2788	4.8	62.6	1	100.00	15.5	even	ok
832.2617	1	C33H43N7NaO17	832.2608	-1.2	10.9	1	100.00	15.5	even	ok