

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\CH25_P1-D-7_01_7536.d
Method lc_qtof_directospos.m
Sample Name CH25
Comment Sv: CH3CN + MeOH + HCOOH
Uhrig

Acquisition Date 7/14/2023 3:40:39 PM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

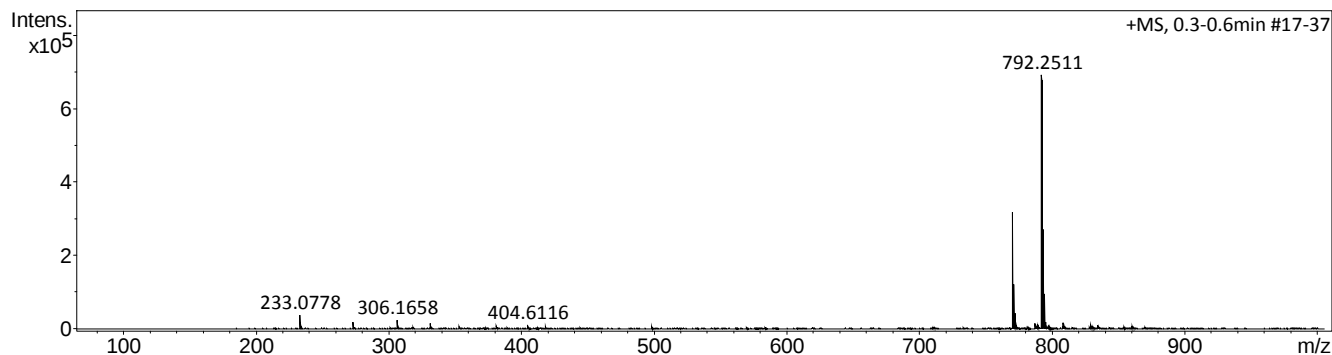

#	m/z	I	I %
1	233.0778	37545	5.4
2	234.0819	5463	0.8
3	273.1013	18187	2.6
4	306.1658	24267	3.5
5	331.2100	14092	2.0
6	353.2645	6141	0.9
7	381.2956	7482	1.1
8	404.6116	10493	1.5
9	418.2879	5681	0.8
10	498.1790	6036	0.9
11	770.2683	316571	45.9
12	771.2725	121633	17.6
13	772.2693	43156	6.3
14	773.2718	9359	1.4
15	787.2974	14511	2.1
16	788.2986	6431	0.9
17	789.2507	11200	1.6
18	789.7472	7978	1.2
19	790.2487	4968	0.7
20	792.2511	690358	100.0
21	793.2533	270293	39.2
22	794.2517	94941	13.8
23	795.2533	18968	2.7
24	797.2339	7813	1.1
25	797.7338	5096	0.7
26	808.2203	16949	2.5
27	809.2264	6035	0.9
28	829.3346	11759	1.7
29	834.2925	9637	1.4
30	860.2365	5454	0.8